


# Appendix D


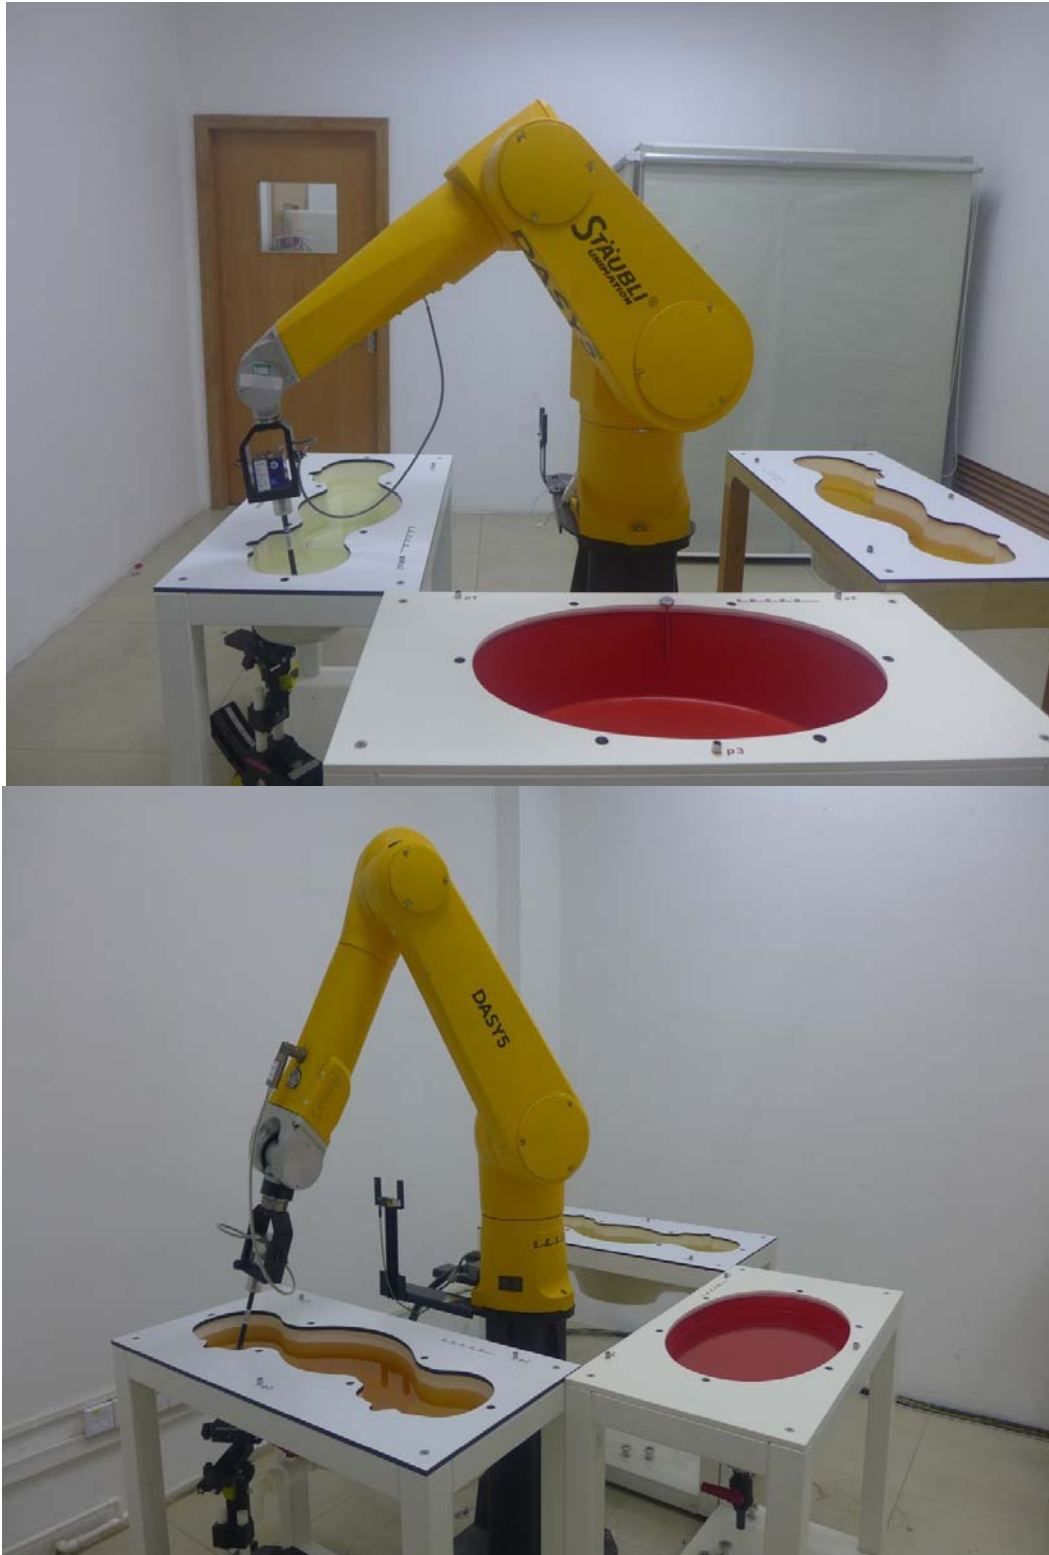


## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


## 1. SAR measurement System



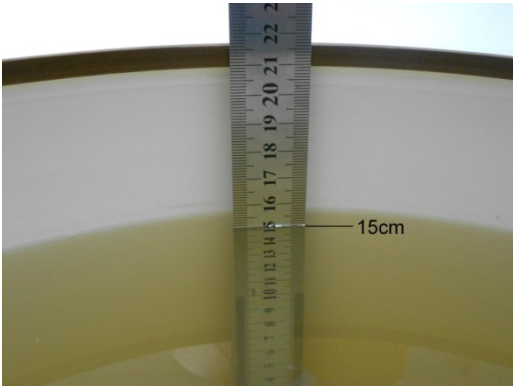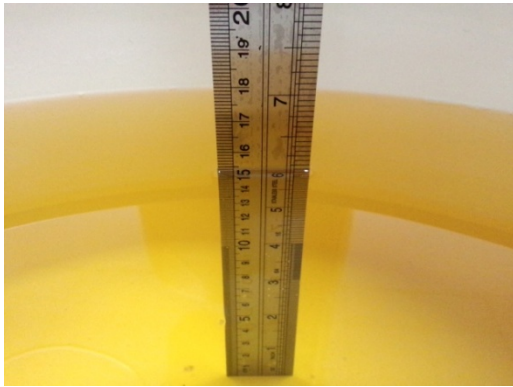

## 2. Photographs of Tissue Simulate Liquid

<b>Photo 1: Tissue Simulant Liquid for Head 835</b>	<b>Photo 2: Tissue Simulant Liquid for Head 1900</b>
	
<b>Photo 3: Tissue Simulant Liquid for Head 2450</b>	<b>Photo 4: Tissue Simulant Liquid for Head 2600</b>
	

### 3. Photographs of EUT test position

Photo 5: Front side 0mm	NA
	<p>NA</p>

## 4. EUT Constructional Details

Photo 6: Front View	Photo 7: Back View
 <p>A small, black, rectangular electronic device is shown from the front. It has a silver-colored metal strip on the left side with two small circular holes. The device is placed on a blue surface next to a ruler for scale. The ruler shows measurements in centimeters, with the device spanning approximately 2.5 cm.</p>	 <p>The back of the device is shown, featuring the 'coolpad' logo and a QR code. The device is placed on a blue surface next to a ruler for scale. The ruler shows measurements in centimeters, with the device spanning approximately 2.5 cm.</p>