

EMC TEST REPORT

FCC 47 CFR Part 15B
Industry Canada ICES-003

Electromagnetic compatibility - Unintentional radiators

Report Reference No. : G0M-1702-6295-EF0115B-SU-V01

Testing Laboratory : Eurofins Product Service GmbH

Address : Storkower Str. 38c
15526 Reichenwalde
Germany

Accreditation :



A2LA Accredited Testing Laboratory, Certificate No.: 1983.01
FCC Filed Test Laboratory, Reg.-No.: 96970
IC OATS Filing assigned code: 3470A

Applicant's name : eResearchTechnology GmbH

Address : Sieboldstrasse 3
97230 Estenfeld
GERMANY

Test specification:

Standard..... : 47 CFR Part 15 Subpart B
ICES-003, Issue 6:2016
ANSI C63.4:2014

Equipment under test (EUT):

| | |
|-----------------------------|--|
| Product description | Spirometer |
| Model No. | SpiroSphere - Sensor Unit |
| Additional Models | None |
| Hardware version | 06.06.00 |
| Firmware / Software version | Firmware µC: 00.12.00 / Bootloader µC: 01.00.00 / BT-Script: 8 |
| | FCC-ID: 2AAUFSPS002 IC: 11335A-SPS002 |

Test result **Passed**

Test Report No.: G0M-1702-6295-EF0115B-SU-V01

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

Possible test case verdicts:

- not applicable to test object: N/A
- test object does meet the requirement.....: P (Pass)
- test object does not meet the requirement.....: F (Fail)

Testing:

Date of receipt of test item: 2017-03-24

Date (s) of performance of tests: 2017-04-07 – 2017-04-21

Compiled by: Marco Belz

Tested by (+ signature).....: Andreas Pflug/Marco Belz

Approved by (+ signature): Jens Marquardt
Deputy Head of Lab

Date of issue: 2017-05-19

Total number of pages.....: 28


General remarks:

The test results presented in this report relate only to the object tested.

The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

Additional comments:

Version History

| Version | Issue Date | Remarks | Revised by |
|---------|------------|-----------------|------------|
| V01 | 2017-05-12 | Initial Release | |



REPORT INDEX

| | | |
|----------|---|-----------|
| 1 | EQUIPMENT (TEST ITEM) DESCRIPTION | 5 |
| 1.1 | Photos – Equipment external | 6 |
| 1.2 | Photos – Equipment internal | 8 |
| 1.3 | Photos – Test setup | 10 |
| 1.4 | Supporting Equipment Used During Testing | 12 |
| 1.5 | Input / Output Ports | 12 |
| 1.6 | Operating Modes and Configurations | 13 |
| 1.7 | Test Equipment Used During Testing | 14 |
| 1.8 | Sample emission level calculation | 15 |
| 2 | RESULT SUMMARY | 16 |
| 3 | TEST CONDITIONS AND RESULTS | 17 |
| 3.1 | Test Conditions and Results – Radiated emissions | 17 |
| 3.2 | Test Conditions and Results – AC power line conducted emissions | 25 |

1 Equipment (Test item) Description



| | |
|------------------------------------|--|
| Description | Spirometer |
| Model | SpiroSphere - Sensor Unit |
| Additional Models | None |
| Serial number | 00000022 |
| Hardware version | 06.06.00 |
| Software / Firmware version | Firmware μ C: 00.12.00 / Bootloader μ C: 01.00.00 / BT-Script: 8 |
| FCC-ID | 2AAUFSPS002 |
| IC | 11335A-SPS002 |
| Power supply | 3.7 VDC via internal Battery |
| Manufacturer | eResearchTechnology GmbH Sieboldstrasse 3 97230 Estenfeld GERMANY |
| Highest emission frequency | fmax [MHz] = 2400 |
| Device classification | Class B |
| Equipment type | Tabletop |
| Number of tested samples | 1 |

1.1 Photos – Equipment external

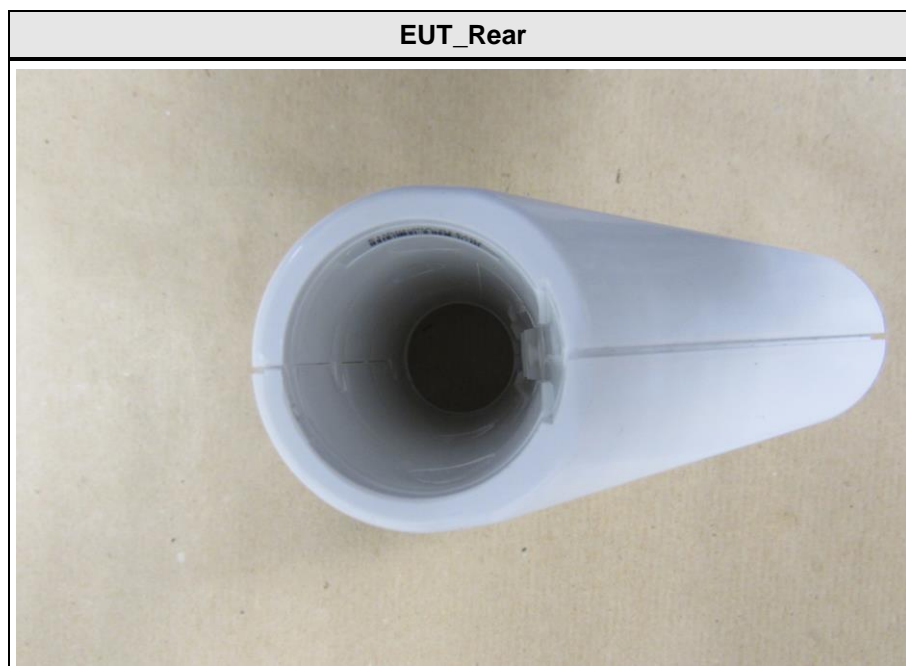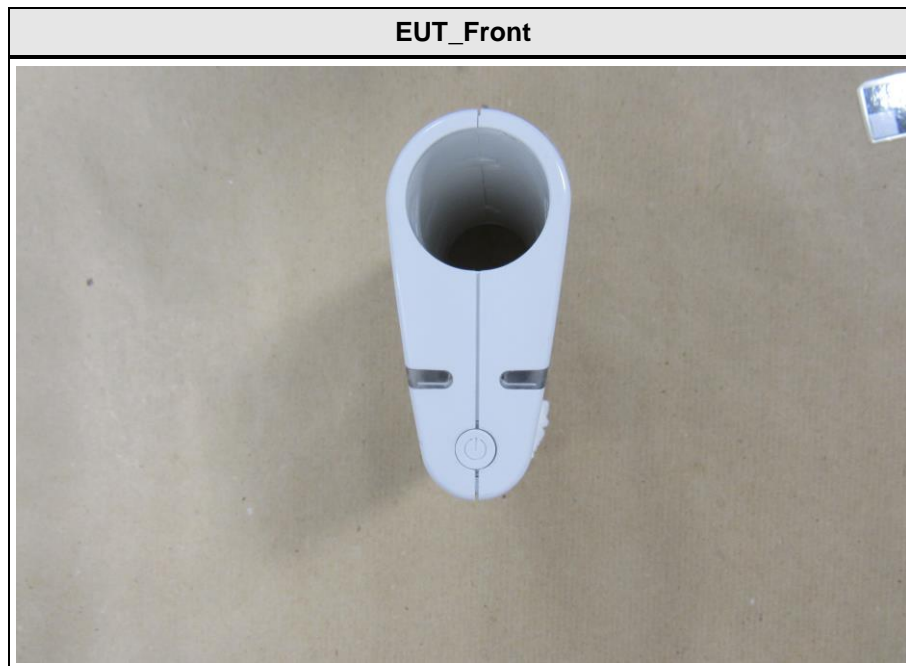



1.2 Photos – Equipment internal

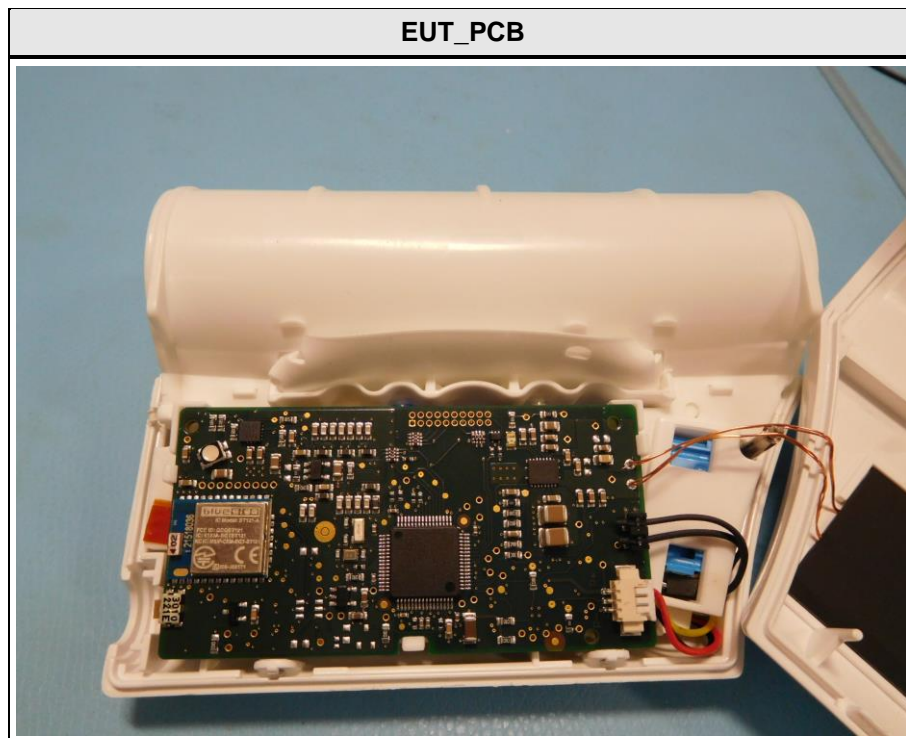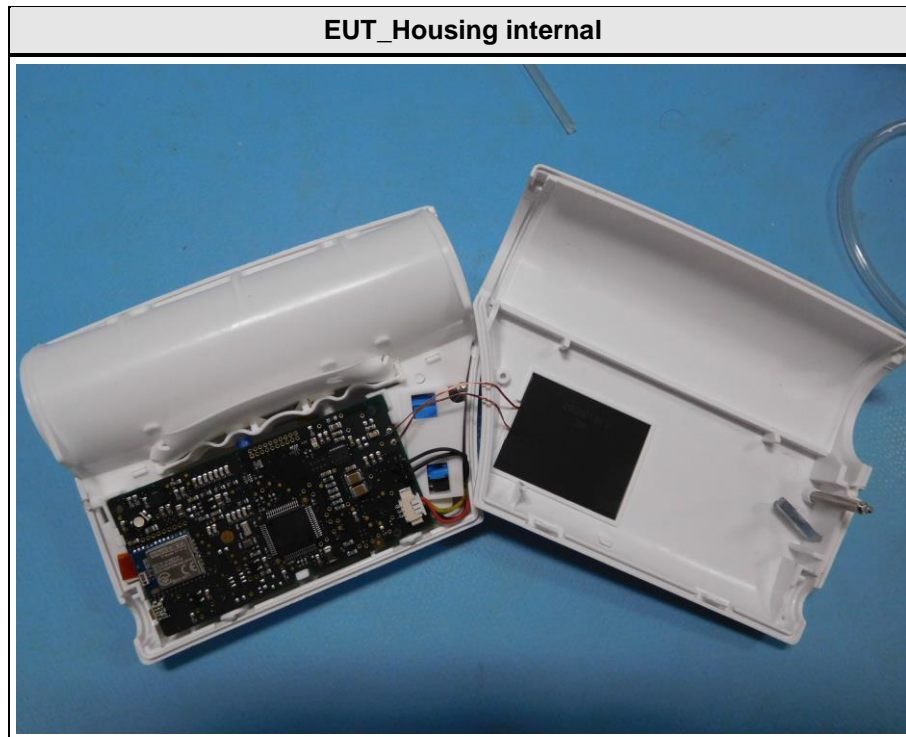



EUT_Radio Module




EUT_Battery



1.3 Photos – Test setup

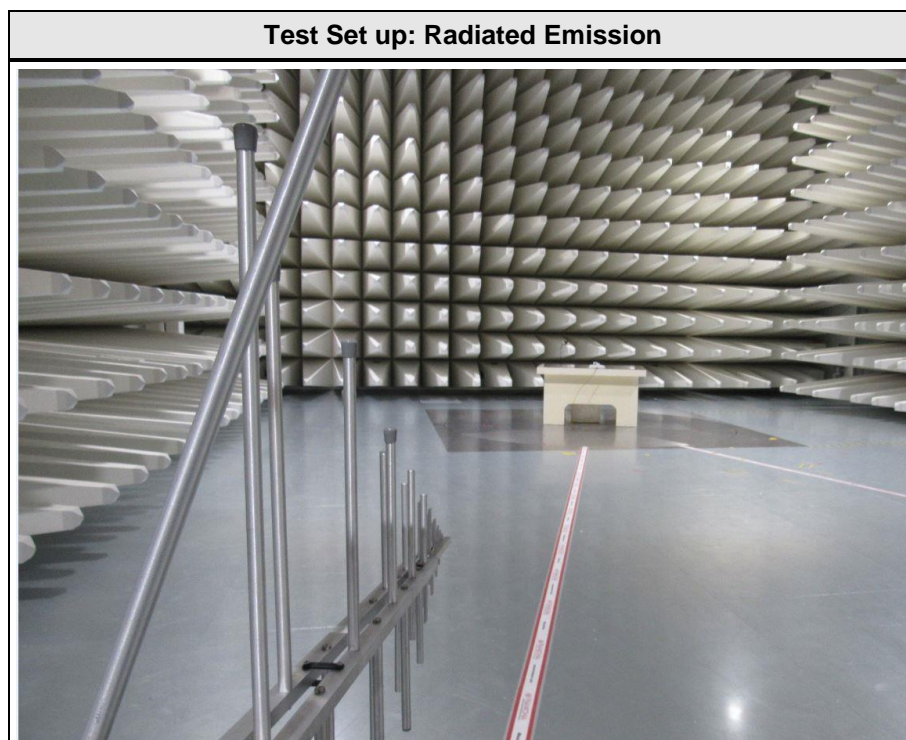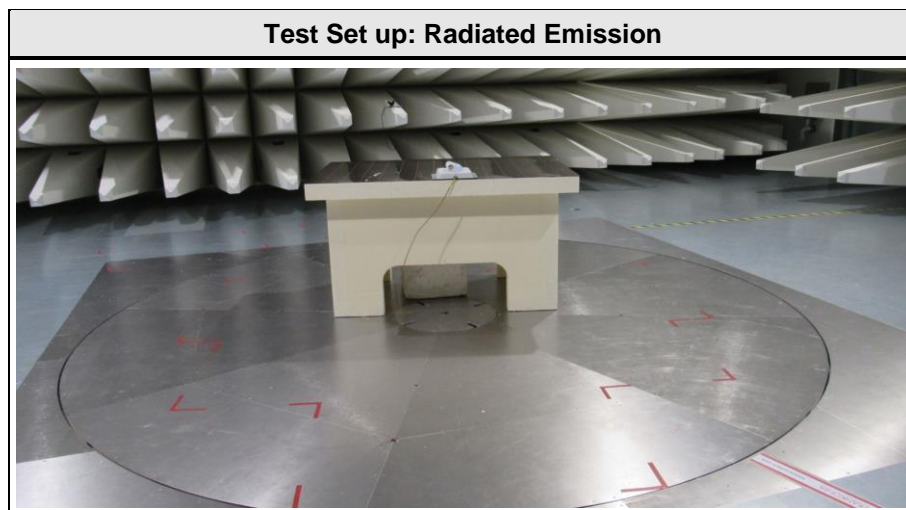

Test Set up: Conducted Emission

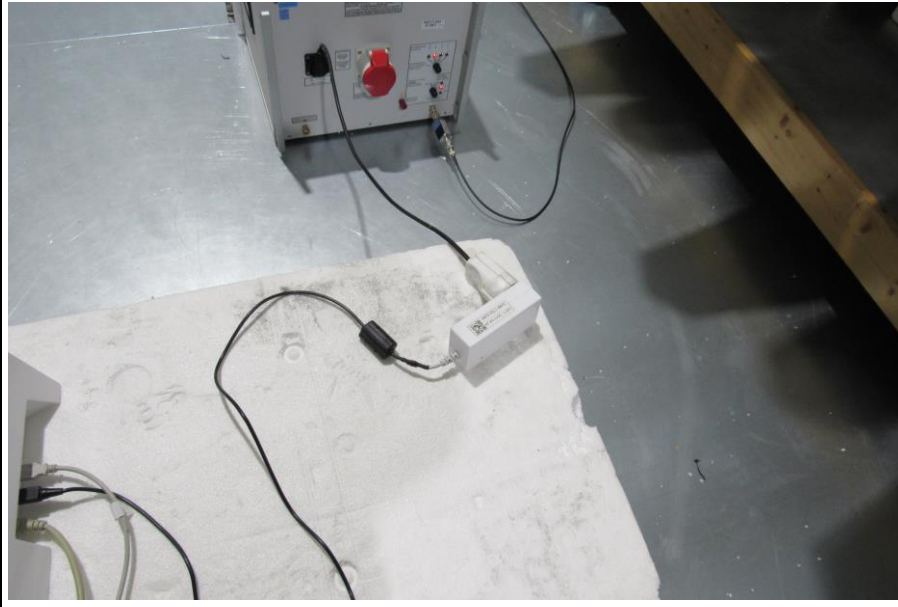

1.4 Supporting Equipment Used During Testing

| Product Type* | Device | Manufacturer | Model No. | Comments (e.g. serial no.) |
|---------------|---------------|--------------|----------------------|----------------------------|
| AE | MainUnit | eResearch | SpiroSphere | 00000053 |
| AE | AC/DC Adapter | Globtek | GTM91099-3009-4.0-T2 | RoHS 186826134/16 |
| AE | Notebook | Lenovo | SL510 | Inv. MEXX0173 |

***Note:** Use the following abbreviations:

AE : Auxiliary/Associated Equipment, or

SIM : Simulator (Not Subjected to Test)

CABL : Connecting cables

1.5 Input / Output Ports

| Port # | Name | Type* | Max. Cable Length | Cable Shielded | Comments (e.g. Cat. of Cable) |
|--------|------|-------|-------------------|----------------|-------------------------------|
| - | - | - | - | - | - |

***Note:** Use the following abbreviations:

AC : AC power port

DC : DC power port

N/E : Non electrical

I/O : Signal input or output port

TP : Telecommunication port

1.6 Operating Modes and Configurations

| Mode # | Description |
|--------|--|
| 1 | Bluetooth-Connection active; continuous measurement; |
| 2 | Charging |

| Configuration # | EUT Configuration |
|-----------------|---|
| 1 | SensorUnit was paired with MainUnit via Bluetooth |
| 2 | SensorUnit was placed in MainUnit for charging |

1.7 Test Equipment Used During Testing

| Measurement Software | | | |
|----------------------|------------------|------------|-----------|
| Description | Manufacturer | Name | Version |
| EMC Test Software | Dare Instruments | Radimation | 2016.1.10 |

| Conducted emissions SR1 | | | | | |
|-------------------------|--------------|---------|------------|-------------|-------------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| AMN | R&S | ESH2-Z5 | EF00182 | | |
| AMN | R&S | ESH3-Z5 | EF00036 | | |
| EMI Test Receiver | R&S | ESR7 | EF00943 | | |
| Cable | - | RG223/U | - | System Cal. | System Cal. |

| Radiated emissions AC1 | | | | | |
|------------------------|-----------------------|----------------|------------|-------------|------------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| Biconical Antenna | R&S | HK 116 | EF00030 | | |
| LPD Antenna | R&S | HL 223 | EF00187 | | |
| Horn antenna | Schwarzbeck | BBHA 9120D | EF00018 | | |
| MXE EMI Receiver | Keysight Technologies | N9038A-526/WXP | EF01070 | | |
| RF Cable | | | - | System Cal. | System Cal |
| RF Cable | | | - | System Cal. | System Cal |

| Conducted emissions AC6 | | | | | |
|-------------------------|--------------------------------|-----------|------------|-------------|-------------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| LISN | Schwarzbeck | NSLK 8128 | EF00975 | | |
| EMI Test Receiver | Rohde & Schwarz Vertriebs GmbH | ESU26 | EF00887 | | |
| Pulse Limiter | R&S | ESH3-Z2 | EF01063 | | |
| Cable | - | RG223/U | - | System Cal. | System Cal. |

| Radiated emissions AC6 | | | | | |
|-----------------------------|----------------|---------------|------------|-------------|------------|
| Description | Manufacturer | Model | Identifier | Cal. Date | Cal. Due |
| TRILOG Broadband Antenna | Schwarzbeck | VULB 9162 | EF00978 | | |
| Double-Ridged Guide Antenna | ETS-Lindgren | 3117 | EF00976 | | |
| EMI Test Receiver | R&S | ESU26 | EF00887 | | |
| RF Cable | Huber & Suhner | Sucoflex 106 | - | System Cal. | System Cal |
| RF Cable | Huber & Suhner | Multiflex 141 | - | System Cal. | System Cal |

Test Report No.: G0M-1702-6295-EF0115B-SU-V01

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

1.8 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dBμV. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dBμV/m). The FCC limits are given in units of μV/m. The following formula is used to convert the units of μV/m to dBμV/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

| | | | | | | | | |
|-----------|---|-------|---|-------------|---|---------------------------|---|---------|
| Reading | + | AF | = | Net Reading | : | Net reading - FCC limit | = | Margin |
| 21.5 dBμV | + | 26 dB | = | 47.5 dBμV/m | : | 47.5 dBμV/m - 57.0 dBμV/m | = | -9.5 dB |

2 Result Summary

| FCC 47 CFR Part 15B, Industry Canada ICES-003 | | | | |
|---|-----------------------------------|------------------|--------|---------|
| Product Specific Standard | Requirement – Test | Reference Method | Result | Remarks |
| 47 CFR 15.109 ICES-003 Item 6.2 | Radiated emissions | ANSI C 63.4 | PASS | |
| 47 CFR 15.107 ICES-003 Item 6.1 | AC power line conducted emissions | ANSI C63.4 | PASS | |
| Remarks: | | | | |

3 Test Conditions and Results

3.1 Test Conditions and Results – Radiated emissions

| Radiated emissions acc. FCC 47 CFR 15.109 / ICES-003 | | | | Verdict: PASS | | |
|--|---------------------|----------------------------|------------------|-----------------|---------------|--------|
| Laboratory Parameters: | | Required prior to the test | | During the test | | |
| Ambient Temperature | | 15 to 35 °C | | 22 °C +/- 2 K | | |
| Relative Humidity | | 30 to 60 % | | 34 % +/- 3 % | | |
| Test according referenced standards | | Reference Method | | | | |
| | | ANSI C63.4 | | | | |
| Sample is tested with respect to the requirements of the equipment class | | Equipment class | | | | |
| | | Class B | | | | |
| Test frequency range determined from highest emission frequency | | Highest emission frequency | | | | |
| | | Fmax [MHz] = 2400 | | | | |
| Fully configured sample scanned over the following frequency range | | Frequency range | | | | |
| | | 30 MHz to 15 GHz | | | | |
| Operating mode | | 1 / 2 | | | | |
| Configuration | | 1 / 2 | | | | |
| Limits and results Class B | | | | | | |
| Frequency [MHz] | Quasi-Peak [dBµV/m] | Result | Average [dBµV/m] | Result | Peak [dBµV/m] | Result |
| 30 – 88 | 40 | PASS | - | | - | - |
| 88 – 216 | 43.5 | PASS | - | | - | - |
| 216 – 960 | 46 | PASS | - | | - | - |
| 960 – 1000 | 54 | PASS | - | | - | - |
| > 1000 | - | - | 54 | PASS | 74 | PASS |
| Comments: | | | | | | |

Test Procedure:

The test site is in accordance with ANSI C63-4:2014 requirements and is listed by FCC.

The measurement procedure is as follows:

Exploratory measurement:

- The EUT was placed on a non-conductive table at a height of 0.8m.
- The EUT and support equipment, if needed, were set up to simulate typical usage.
- Cables, of type and length specified by the manufacturer, were connected to at least one port of each type and were terminated by a device or simulating load of actual usage.
- The antenna was placed at a distance of 3 or 10 m.
- The received signal was monitored at the measurement receiver.
 - Cables not bundled were manipulated within the range of likely arrangements to produce the highest emission amplitude
 - To maximize the suspected emissions the EUT is rotated 360 degrees. If the signal exceeds the previous amplitude, go back to the corresponding azimuth and manipulate the cables again for maximizing the emissions if possible.
 - Move the antenna from 1 to 4m to maximize the suspected highest amplitude signal.
- This procedure has to be performed in both antenna polarizations, horizontal and vertical.
- The arrangement of the equipment with the maximum emission level is shown on the setup picture at item 1.3.

Final measurement:


- The EUT was placed on a 0.8 m non-conductive table at a 3 m distance from the receive antenna. The antenna output was connected to the measurement receiver
- A biconical antenna was used for the frequency range 30 – 200 MHz, a logarithmic periodical antenna was used for the frequency range from 200 – 1000 MHz. Above one 1 GHz a Double Ridged Broadband Horn antenna was used. The antenna was placed on an adjustable height antenna mast
- The EUT and cable arrangement were based on the exploratory measurement results
- Emissions were maximized at each frequency by rotating the EUT and adjusting the receive antenna height and polarization. The maximum values were recorded.
- The test data of the worst-case conditions were recorded and shown on the next pages.

Radiated emissions according to FCC 15B

Project number: G0M-1702-6295

| | |
|-----------------------|---------------------------------|
| Applicant: | eResearchTechnology GmbH |
| EUT Name: | Spirometer |
| Model: | SpiroSphere - Sensor Unit |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Belz |
| Test Conditions: | Tnom: 22°C, Unom: 120 VAC 60 Hz |
| Antenna: | Schwarzbeck VULB 9162, Vertical |
| Measurement distance: | 3 m |
| Mode: | 1 |
| Test Date: | 2017-04-18 |
| Note: | |

Index 12

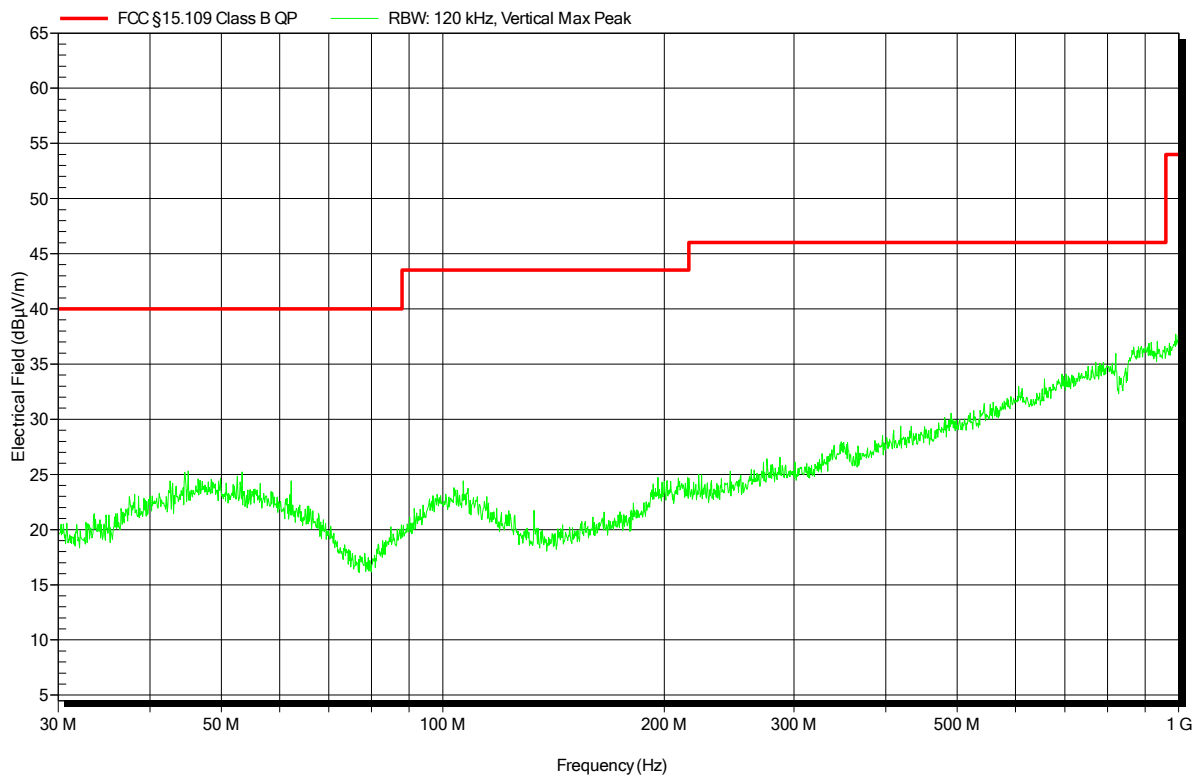


Radiated emissions according to FCC 15B

Project number: G0M-1702-6295

| | |
|-----------------------|-----------------------------------|
| Applicant: | eResearchTechnology GmbH |
| EUT Name: | Spirometer |
| Model: | SpiroSphere - Sensor Unit |
| Test Site: | Eurofins Product Service GmbH |
| Operator: | Mr. Belz |
| Test Conditions: | Tnom: 22°C, Unom: 120 VAC 60 Hz |
| Antenna: | Schwarzbeck VULB 9162, Horizontal |
| Measurement distance: | 3 m |
| Mode: | 1 |
| Test Date: | 2017-04-18 |
| Note: | |

Index 13

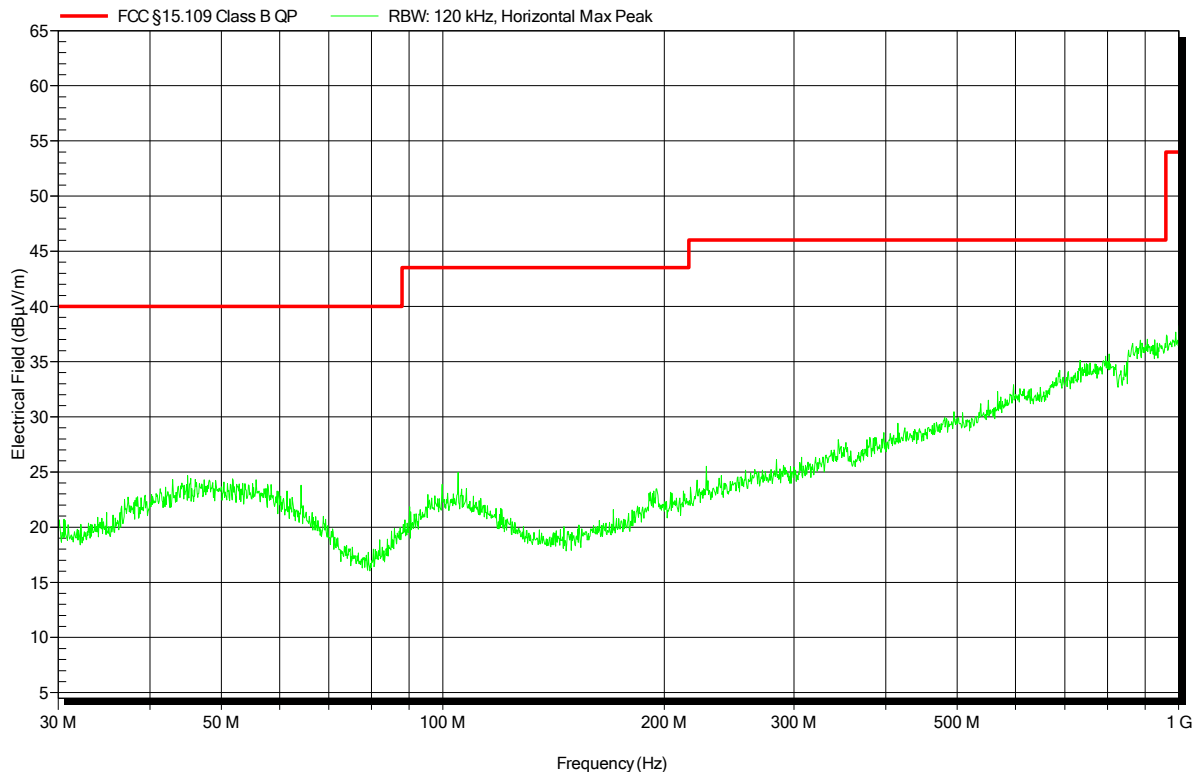


Radiated emissions according to FCC 15B

Project number: G0M-1702-6295

Applicant: eResearchTechnology GmbH
EUT Name: Spirometer
Model: SpiroSphere - Sensor Unit
Test Site: Eurofins Product Service GmbH
Operator: Mr. Belz
Test Conditions: Tnom: 22°C, Unom: 120 VAC 60 Hz
Antenna: Schwarzbeck VULB 9162, Vertical
Measurement distance: 3 m
Mode: 2
Test Date: 2017-04-18
Note:

Index 17

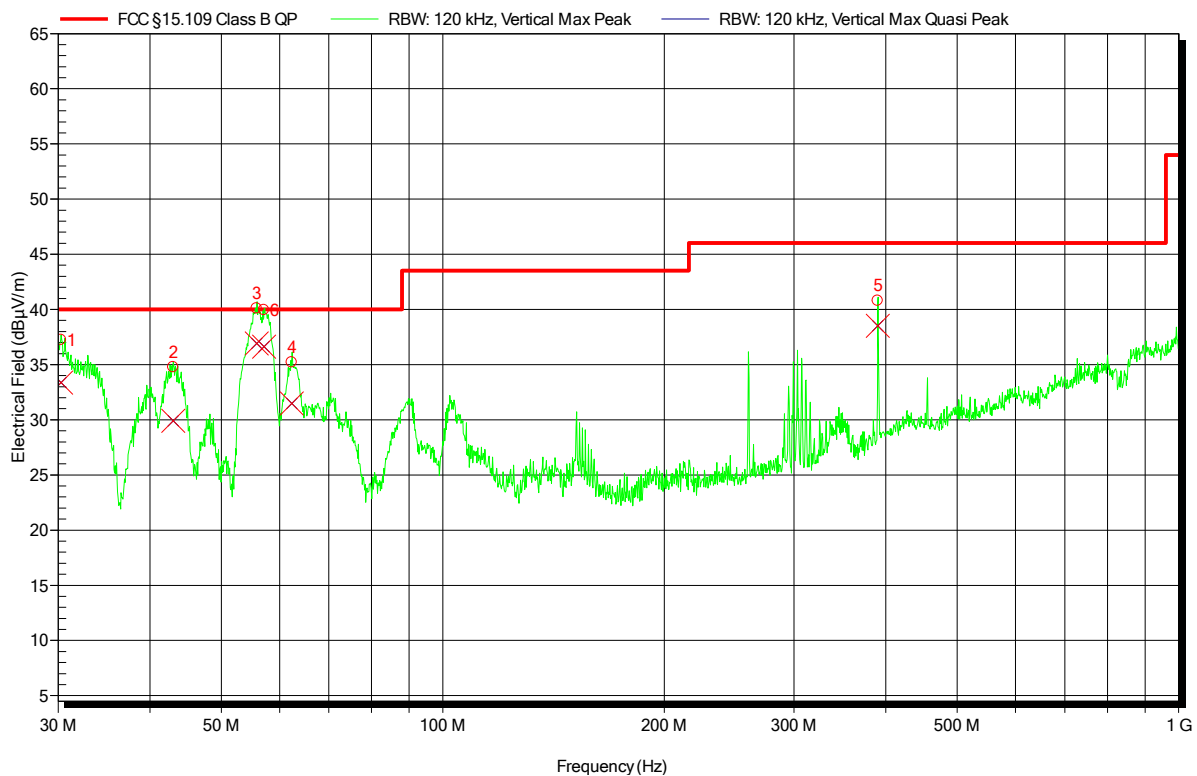

| Peak Number | Frequency | Quasi-Peak | Quasi-Peak Limit | Quasi-Peak Difference | Quasi-Peak Status | Angle | Height |
|-------------|-------------|-------------|------------------|-----------------------|-------------------|----------|--------|
| 1 | 30.3 MHz | 33.4 dBμV/m | 40 dBμV/m | -6.6 dB | Pass | 0 Degree | 1 m |
| 2 | 43.02 MHz | 29.9 dBμV/m | 40 dBμV/m | -10.1 dB | Pass | 0 Degree | 1 m |
| 3 | 55.86 MHz | 36.9 dBμV/m | 40 dBμV/m | -3.1 dB | Pass | 0 Degree | 1 m |
| 4 | 62.34 MHz | 31.5 dBμV/m | 40 dBμV/m | -8.5 dB | Pass | 0 Degree | 1 m |
| 5 | 389.982 MHz | 38.5 dBμV/m | 46 dBμV/m | -7.5 dB | Pass | 0 Degree | 1 m |
| 6 | 57.18 MHz | 36.6 dBμV/m | 40 dBμV/m | -3.4 dB | Pass | 0 Degree | 1 m |

Test Report No.: G0M-1702-6295-EF0115B-SU-V01


Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated emissions according to FCC 15B

Project number: G0M-1702-6295

Applicant: eResearchTechnology GmbH
EUT Name: Spirometer
Model: SpiroSphere - Sensor Unit
Test Site: Eurofins Product Service GmbH
Operator: Mr. Belz
Test Conditions: Tnom: 22°C, Unom: 120 VAC 60 Hz
Antenna: Schwarzbeck VULB 9162, Horizontal
Measurement distance: 3 m
Mode: 1
Test Date: 2017-04-18
Note:

Index 18

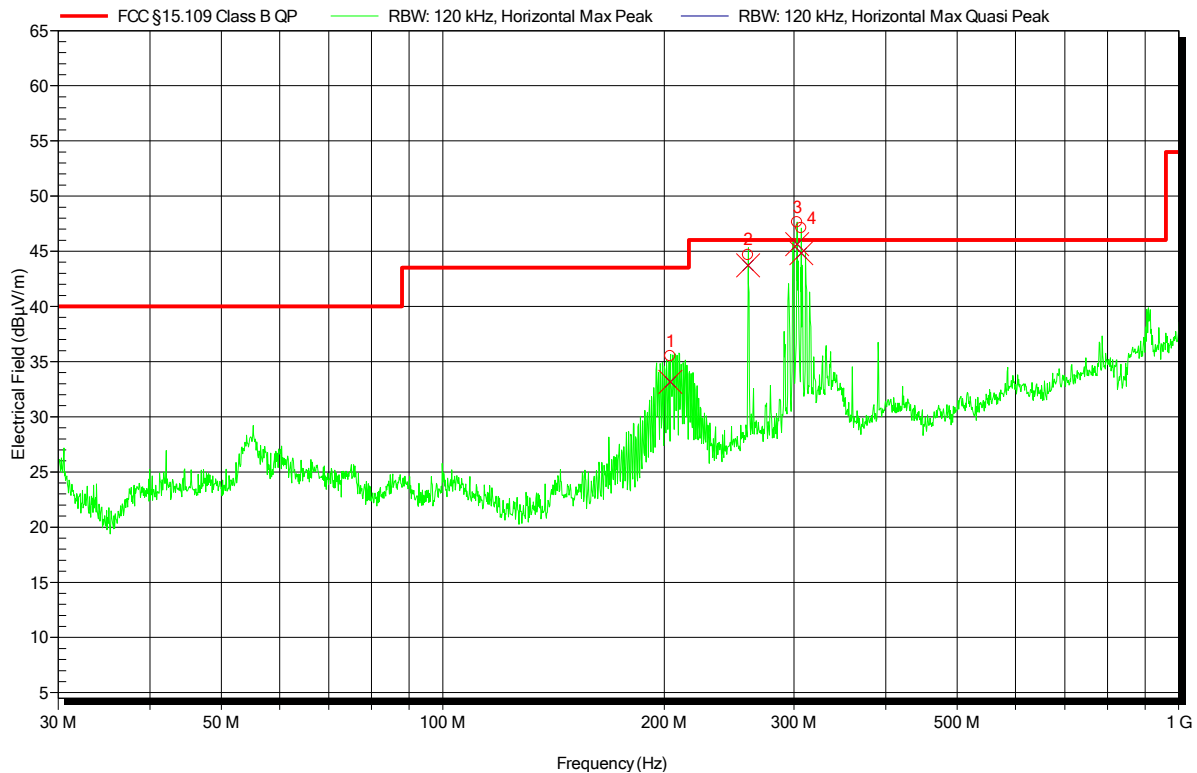


| Peak Number | Frequency | Quasi-Peak | Quasi-Peak Limit | Quasi-Peak Difference | Quasi-Peak Status | Angle | Height |
|-------------|-------------|-------------|------------------|-----------------------|-------------------|----------|--------|
| 1 | 203.832 MHz | 33.2 dBμV/m | 43.5 dBμV/m | -10.3 dB | Pass | 0 Degree | 3.7 m |
| 2 | 259.974 MHz | 43.7 dBμV/m | 46 dBμV/m | -2.3 dB | Pass | 0 Degree | 3.7 m |
| 3 | 302.874 MHz | 45.7 dBμV/m | 46 dBμV/m | -0.4 dB | Pass | 0 Degree | 3.7 m |
| 4 | 306.96 MHz | 44.8 dBμV/m | 46 dBμV/m | -1.2 dB | Pass | 0 Degree | 3.7 m |

Radiated emissions according to FCC 15B

Project number: GOM-1702-6295

Applicant: eResearchTechnology GmbH
 EUT Name: Spirometer
 Model: SpiroSphere - Sensor Unit
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Belz
 Test Conditions: Tnom: 22°C, Unom: 120 VAC 60 Hz
 Antenna: ETS-Lindgren 3117, Vertical
 Measurement distance: 3 m
 Mode: 1
 Test Date: 2017-04-21
 Note:

Index 34

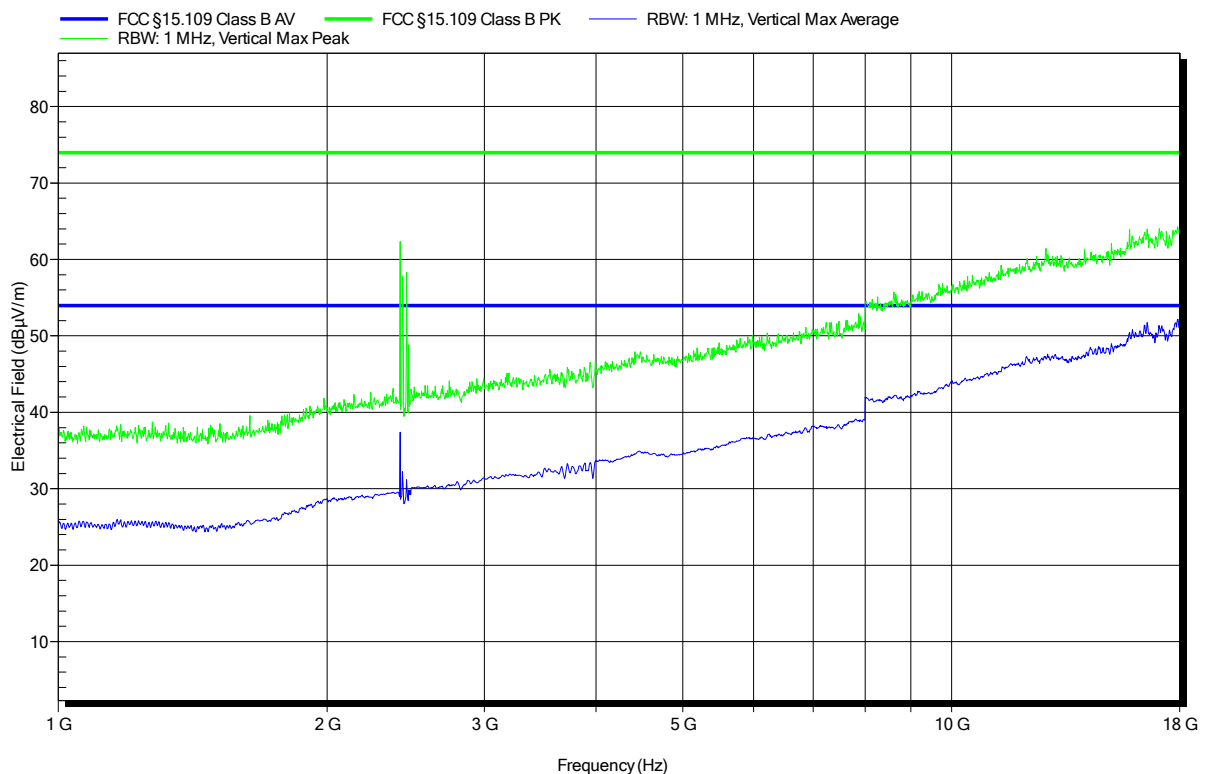


Radiated emissions according to FCC 15B

Project number: G0M-1702-6295

Applicant: eResearchTechnology GmbH
 EUT Name: Spirometer
 Model: SpiroSphere - Sensor Unit
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Belz
 Test Conditions: Tnom: 22°C, Unom: 120 VAC 60 Hz
 Antenna: ETS-Lindgren 3117, Horizontal
 Measurement distance: 3 m
 Mode: 1
 Test Date: 2017-04-21
 Note:

Index 35

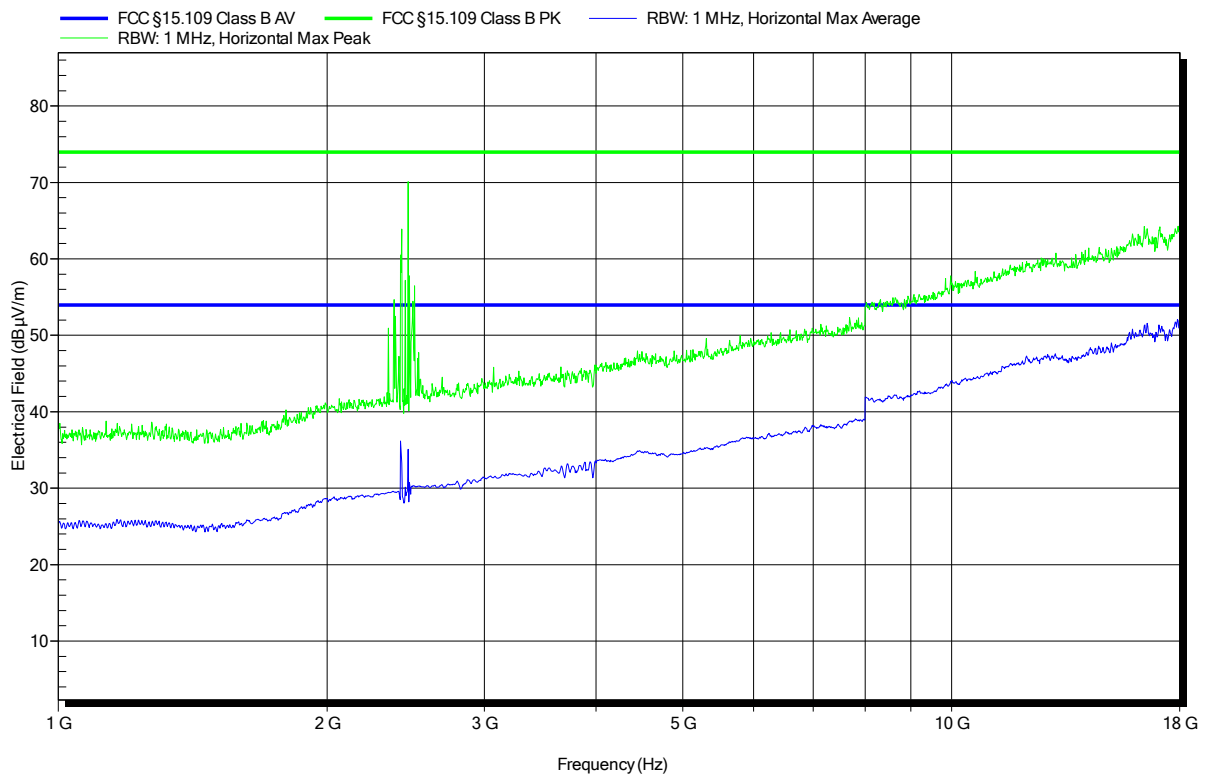

Test Report No.: G0M-1702-6295-EF0115B-SU-V01

Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

3.2 Test Conditions and Results – AC power line conducted emissions

| Conducted emissions acc. FCC 47 CFR 15.107 / ICES-003 | | | Verdict: PASS | |
|--|----------------------------|--------|-----------------|--------|
| Laboratory Parameters: | Required prior to the test | | During the test | |
| Ambient Temperature | 15 to 35 °C | | 22 °C +/- 2 K | |
| Relative Humidity | 30 to 60 % | | 34 % +/- 3 % | |
| Test according referenced standards | Reference Method | | | |
| | ANSI C63.4 | | | |
| Fully configured sample scanned over the following frequency range | Frequency range | | | |
| | 0.15 MHz to 30 MHz | | | |
| Sample is tested with respect to the requirements of the equipment class | Equipment class | | | |
| | Class B | | | |
| Points of Application | Application Interface | | | |
| AC Mains | LISN | | | |
| Operating mode | 2 | | | |
| Configuration | 2 | | | |
| Limits and results Class B | | | | |
| Frequency [MHz] | Quasi-Peak [dBµV] | Result | Average [dBµV] | Result |
| 0.15 to 5 | 66 to 56* | PASS | 56 to 46* | PASS |
| 0.5 to 5 | 56 | PASS | 46 | PASS |
| 5 to 30 | 60 | PASS | 50 | PASS |
| Comments: | | | | |
| * Limit decreases linearly with the logarithm of the frequency. | | | | |

Test Procedure:

The test site is in accordance with ANSI C63-4:2014 requirements and is listed by FCC.

The measurement procedure is as follows:

Exploratory measurement:

- The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1)
- The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN.
- The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length).
- The LISN measurement port was connected to a measurement receiver
- I/O cables were bundled not longer than 0.4 m
- Measurement was performed in the frequency range 0.15 – 30MHz on each current-carrying conductor
- To maximize the emissions the cable positions were manipulated
- The worst configuration of EUT and cables is shown on a test setup picture at item 1.3

Test Procedure:

Final measurement:


- The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1)
- The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN.
- The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length).
- The LISN measurement port was connected to a measurement receiver
- The EUT and cable arrangement were based on the exploratory measurement results
- The test data of the worst-case conditions were recorded and shown on the next pages.

Conducted emissions according to FCC 15b

Project number: G0M-1702-6295

Applicant: eResearchTechnology GmbH
 EUT Name: Spirometer
 Model: SpiroSphere - Sensor Unit
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Belz
 Test Conditions: Tnom: 22°C, Unom: 120 VAC
 LISN: Schwarzbeck NSLK 8128 (N)
 Mode: 2
 Test Date: 2017-04-20
 Note:

Index 19

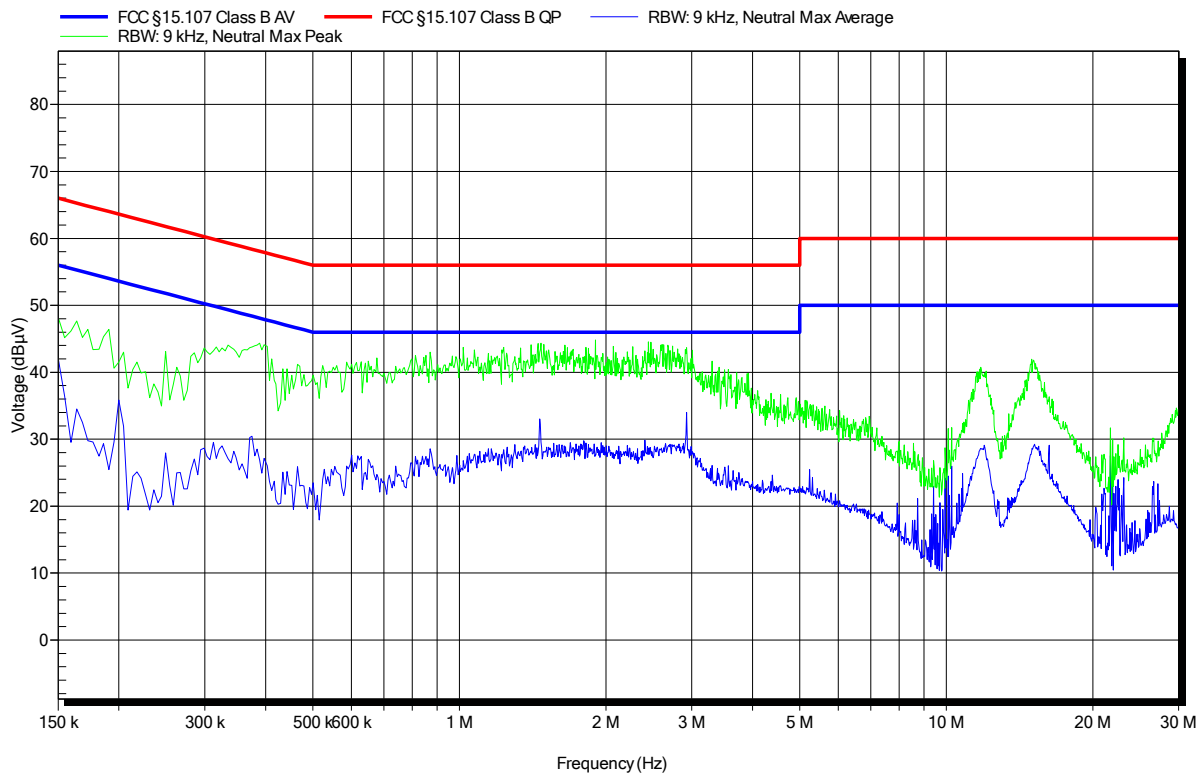

Test Report No.: G0M-1702-6295-EF0115B-SU-V01

Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Conducted emissions according to FCC 15b

Project number: G0M-1702-6295

Applicant: eResearchTechnology GmbH
 EUT Name: Spirometer
 Model: SpiroSphere - Sensor Unit
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Belz
 Test Conditions: Tnom: 22°C, Unom: 120 VAC
 LISN: Schwarzbeck NSLK 8128 (L)
 Mode: 2
 Test Date: 2017-04-20
 Note:

Index 20

