

Appendix D

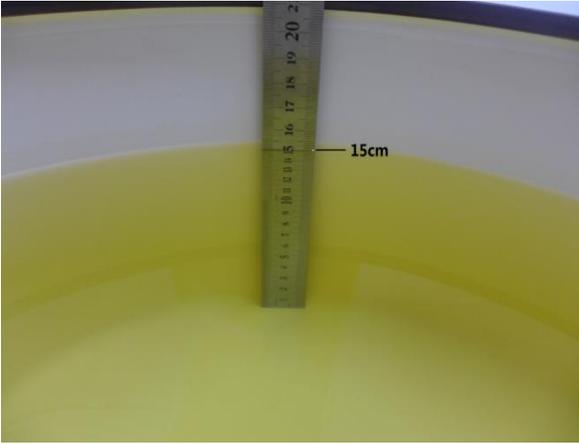
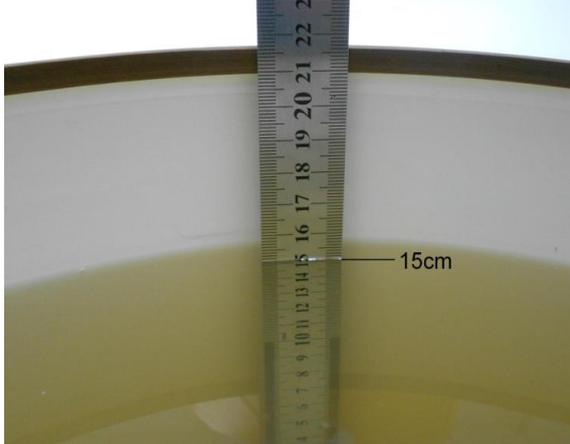
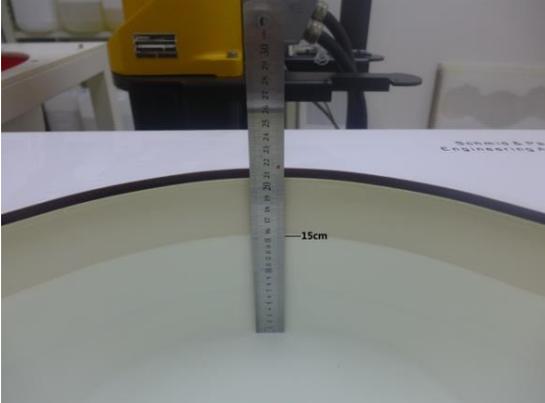
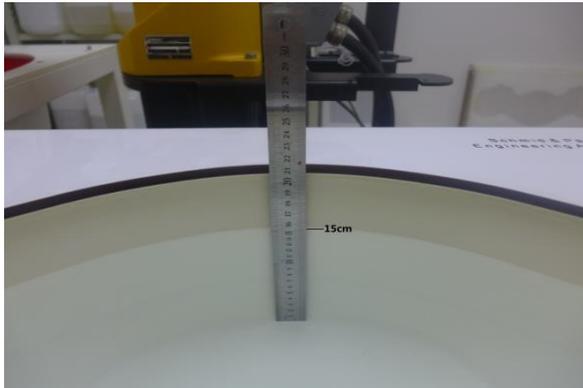
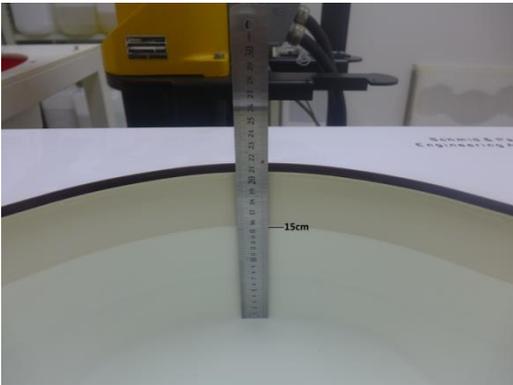
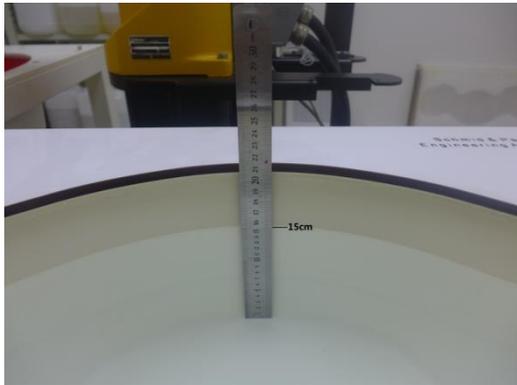
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

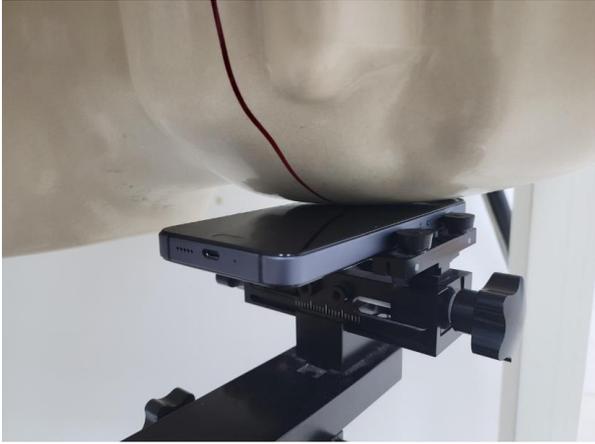
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1800</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5GHz</p>
	

3. Photographs of EUT test position

<p>Photo 7: Left cheek 0mm</p>	<p>Photo 8: Right cheek 0mm</p>
	
<p>Photo 9: Front side 10mm</p>	<p>Photo 10: Back side 10mm</p>
	
<p>Photo 11: Top side 10mm</p>	
	

4. EUT Constructional Details

Details please Refer to Appendix -

Photographs of EUT Constructional Details for SZCR2109023127AT.