



TEST REPORT

Test Report No. : UL-RPT-RP13754225-416A

Customer : VEGA Grieshaber KG
Model No. : VEGAPULS 6X
FCC ID : O6QPS6XW
Technology : Tank Level Probing Radar
Test Standard(s) : FCC Parts 15.31(q), 15.207 & 15.209(a)
Test Laboratory : UL International (UK) Ltd, Basingstoke, Hampshire, RG24 8AH, United Kingdom

1. This test report shall not be reproduced except in full, without the written approval of UL International (UK) Ltd.
2. The results in this report apply only to the sample(s) tested.
3. The sample tested is in compliance with the above standard(s).
4. The test results in this report are traceable to the national or international standards.
5. Version 1.0.

Date of Issue: 30 November 2021

Checked by:

Sarah Williams
RF Operations Leader, Radio Laboratory

Company Signatory:

Ben Mercer
Lead Project Engineer, Radio Laboratory



5772

UL International (UK) LTD

Unit 1-3 Horizon, Kingsland Business Park, Wade Road, Basingstoke, Hampshire, RG24 8AH, UK
Telephone: +44 (0)1256 312000
Facsimile: +44 (0)1256 312001

Customer Information

Company Name:	VEGA Grieshaber KG
Address:	Am Hohenstein 113 D-77761 Schiltach Germany

Report Revision History

Version Number	Issue Date	Revision Details	Revised By
1.0	30/11/2021	Initial Version	Sarah Williams

Table of Contents

Customer Information.....	2
Report Revision History	2
Table of Contents.....	3
1 Attestation of Test Results.....	4
1.1 Description of EUT	4
1.2 General Information	4
1.3 Summary of Test Results	4
1.4 Deviations from the Test Specification	4
2 Summary of Testing.....	5
2.1 Facilities and Accreditation	5
2.2 Methods and Procedures	5
2.3 Calibration and Uncertainty	6
2.4 Test and Measurement Equipment	7
3 Equipment Under Test (EUT)	9
3.1 Identification of Equipment Under Test (EUT)	9
3.2 Modifications Incorporated in the EUT	9
3.3 Additional Information Related to Testing	9
3.4 Description of Available Antennas	9
3.5 Description of Test Setup	10
4 Radiated Test Results.....	14
4.1 Transmitter Radiated Emissions <1 GHz	14
4.2 Transmitter Radiated Emissions >1 GHz	16
5 AC Power Line Conducted Emissions Test Results.....	25
5.1 Transmitter AC Conducted Spurious Emissions	25

1 Attestation of Test Results





1.1 Description of EUT

The equipment under test was a radar sensor for the continuous level measurement of liquids.

1.2 General Information

Specification Reference:	47CFR15.31
Specification Title:	Code of Federal Regulations Volume 47 (Telecommunications): Part 15 Subpart A (General) – Section 15.31
Specification Reference:	47CFR15.207 and 47CFR15.209
Specification Title:	Code of Federal Regulations Volume 47 (Telecommunications): Part 15 Subpart C (Intentional Radiators) – Sections 15.207 & 15.209
Site Registration:	685609
Lab Designation No.:	UK2011
Location of Testing:	Unit 3 Horizon, Wade Road, Kingsland Business Park, Basingstoke, Hampshire, RG24 8AH, United Kingdom
Test Dates:	14 August 2021 to 05 October 2021

1.3 Summary of Test Results

FCC Reference (47CFR)	Measurement	Result
Part 15.31(q) & 15.209(a)	Transmitter Radiated Emissions	
Part 15.207	Transmitter AC Conducted Emissions	
Key to Results  = Complied  = Did not comply		

1.4 Deviations from the Test Specification

For the measurements contained within this test report, there were no deviations from, additions to, or exclusions from the test specification identified above.

2 Summary of Testing

2.1 Facilities and Accreditation

The test site and measurement facilities used to collect data are located at Unit 3 Horizon, Wade Road, Kingsland Business Park, Basingstoke, Hampshire, RG24 8AH, United Kingdom. The following table identifies which facilities were utilised for radiated emission measurements documented in this report. Specific facilities are also identified in the test results sections.

Site 1	X
Site 2	X
Site 17	X

UL International (UK) Ltd is accredited by the United Kingdom Accreditation Service (UKAS). UKAS is one of the signatories to the International Laboratory Accreditation Co-operation (ILAC) Arrangement for the mutual recognition of test reports. The tests reported herein have been performed in accordance with its terms of accreditation.

2.2 Methods and Procedures

Reference:	ANSI C63.10-2013
Title:	American National Standard of Procedures for Compliance Testing of Unlicensed Wireless Devices
Reference:	KDB 174176 D01 Line Conducted FAQs v01r01
Title:	AC Power-Line Conducted Emissions Frequently Asked Questions

2.3 Calibration and Uncertainty

Measuring Instrument Calibration

In accordance with UKAS requirements all the measurement equipment is on a calibration schedule. All equipment was within the calibration period on the date of testing.

Measurement Uncertainty & Decision Rule

Overview

No measurement or test can ever be perfect and the imperfections give rise to error of measurement in the results. Consequently the result of a measurement is only an approximation to the value of the measurand (the specific quantity subject to measurement) and is only complete when accompanied by a statement of the uncertainty of the approximation.

The expression of uncertainty of a measurement result allows realistic comparison of results with reference values and limits given in specifications and standards.

Decision Rule

The decision rule applied is based upon the accuracy method criteria. The measurement uncertainty is met and the result is considered in conformance with the requirement criteria if the observed value is within the prescribed limit.

Measurement Uncertainty

The reported expanded uncertainties below are based on a standard uncertainty multiplied by an appropriate coverage factor such that a confidence level of approximately 95% is maintained. For the purposes of this document “approximately” is interpreted as meaning “effectively” or “for most practical purposes”.

Measurement Type	Range	Confidence Level (%)	Calculated Uncertainty
Radiated Emissions	9 kHz to 30 MHz	95%	±5.32 dB
Radiated Emissions	30 MHz to 1 GHz	95%	±3.30 dB
Radiated Emissions	1 GHz to 40 GHz	95%	±2.94 dB
Radiated Emissions	40 GHz to 200 GHz	95%	±5.12 dB
Transmitter AC Conducted Emissions	0.15 MHz to 30 MHz	95%	±1.96 dB

The methods used to calculate the above uncertainties are in line with those recommended within the various measurement specifications. Where measurement specifications do not include guidelines for the evaluation of measurement uncertainty the published guidance of the appropriate accreditation body is followed.

2.4 Test and Measurement Equipment

Test Equipment Used for Transmitter Radiated Emissions Tests

Asset No.	Instrument	Manufacturer	Type No.	Serial No.	Date Calibration Due	Cal. Interval (Months)
M2040	Thermohygrometer	Testo	608-H1	45124934	10 Dec 2021	12
K0001	3m RSE Chamber	Rainford EMC	N/A	N/A	06 Sep 2022	12
M2044	Test Receiver	Rohde & Schwarz	ESU26	100122	29 Apr 2022	12
A3198	Loop Antenna	ETS Lindgren	6502	00221887	12 Aug 2022	12
K0017	3m RSE Chamber	Rainford EMC	N/A	N/A	26 Oct 2022	12
M2003	Thermohygrometer	Testo	608-H1	45046641	10 Dec 2021	12
M1874	Test Receiver	Rohde & Schwarz	ESU26	100553	19 May 2022	12
M2077	Test Receiver	Rohde & Schwarz	ESW44	102026	01 Feb 2022	12
A2948	Pre-Amplifier	Com-Power	PAM-118A	551087	20 Oct 2022	12
A2951	Pre-Amplifier	Com-Power	PAM-103	441141	25 Jan 2022	12
A3161	Antenna	Teseq	CBL6111D	50859	04 May 2022	12
A2943	Attenuator	AtlanTecRF	AN18W5-06	208147#2	01 Feb 2022	12
A3265	Pre-Amplifier	Schwarzbeck	BBV 9721	9721-069	03 Nov 2022	12
A2892	Antenna	Schwarzbeck	BBHA 9170	9170-727	02 Nov 2022	12
A2889	Antenna	Schwarzbeck	BBHA 9120 B	00653	26 Oct 2022	12
A2890	Antenna	Schwarzbeck	HWRD 750	014	29 Oct 2022	12
K0002	3m RSE Chamber	Rainford EMC	N/A	N/A	18 Mar 2022	12
M2016	Thermohygrometer	Testo	608-H1	45046428	10 Dec 2021	12
M1794	Spectrum Analyser	Rohde & Schwarz	FSU26	100027	02 Mar 2022	12
G0614	Signal Generator	Rohde & Schwarz	SMB100A	177687	19 May 2023	36
M2064	Downconverter	Virginia Diodes	WR12SAX	SAX 325	17 Feb 2022	24
M2065	Downconverter	Virginia Diodes	WR10SAX	SAX 393	17 Feb 2022	24
M2066	Downconverter	Virginia Diodes	WR6.5SAX	SAX 392	17 Feb 2022	24
M2067	Downconverter	Virginia Diodes	WR4.3SAX	SAX 391	17 Feb 2022	24
M2069	Downconverter	Virginia Diodes	WR15SAX	SAX 394	09 Jul 2023	24
M1621	Harmonic Mixer	Hewlett Packard	11970U	3003A01631	27 May 2024	36
A2963	Antenna	Link Microtek	AM19HA-ULV1	14929	31 Dec 2021	12
A2964	Antenna	Link Microtek	AM15HA-ULV1	14930	31 Dec 2021	12
A2965	Antenna	Link Microtek	AM12HA-ULV1	14931	31 Dec 2021	12
A2967	Antenna	Link Microtek	AM10HA-ULV1	14933	31 Dec 2021	12
A2968	Antenna	Link Microtek	AM7HA-ULV1	14934	31 Dec 2021	12
A2969	Antenna	Link Microtek	AM4HA-ULV1	14935	31 Dec 2021	12

Test and Measurement Equipment (continued)**Test Equipment Used for Transmitter AC Conducted Spurious Emissions:**

Asset No.	Instrument	Manufacturer	Type No.	Serial No.	Date Calibration Due	Cal. Interval (Months)
M2037	Thermohygrometer	Testo	608-H1	45124925	09 Dec 2021	12
A649	LISN	Rohde & Schwarz	ESH3-Z5	82556/008	04 Aug 2022	12
A1830	Pulse Limiter	Rohde & Schwarz	ESH3-Z2	100668	21 Apr 2022	12
M1273	Test Receiver	Rohde & Schwarz	ESIB26	100275	14 Dec 2021	12

Test Measurement Software/Firmware Used:

Name	Version	Release Date
Rohde & Schwarz EMC32	6.30.0	2018

3 Equipment Under Test (EUT)

3.1 Identification of Equipment Under Test (EUT)

Brand Name:	VEGAPULS
Model No.:	VEGAPULS 6X
Test Sample Serial Number:	52403535 (<i>Radiated sample</i>)
Hardware Version:	1.0.0
Software Version:	1.00.00
FCC ID:	O6QPS6XW

3.2 Modifications Incorporated in the EUT

No modifications were applied to the EUT during testing.

3.3 Additional Information Related to Testing

Technology Tested:	Tank Level Probing Radar	
Type of Unit:	Transceiver	
Modulation:	FMCW	
Power Supply Requirement(s):	Nominal	24.0 VDC
Transmit Frequency Range:	75 GHz to 85 GHz	
Transmit Channels Tested:	Channel Bandwidth (GHz)	Channel Frequency (GHz)
	2	79.500
	4	80.000
	8	80.000

3.4 Description of Available Antennas

The radio utilizes various external antennas, with the following maximum gains:

Model Number	Type	Frequency Range (MHz)	Antenna Gain (dBi)
VEGAZW-6-74537	Plastic Horn Antenna	75000 to 85000	34.2
VEGAZW-6-74539	Thread with Integrated Horn Antenna	75000 to 85000	25.3
VEGAZW-6-74547	Flange with Encapsulated Antenna System	75000 to 85000	33.4
VEGAZW-6-74538	Flange with Lens Antenna	75000 to 85000	30.7

3.5 Description of Test Setup

Support Equipment

The following support equipment was used to exercise the EUT during testing:

Description:	Round Nose Pliers
Brand Name:	Belzer
Model Name or Number:	2464-A19
Serial Number:	2051

Description:	240 Litre Tank
Brand Name:	Speidel
Model Name or Number:	Not marked or stated
Serial Number:	Not marked or stated

Description:	DC Power Supply
Brand Name:	ISO-Tech
Model Name or Number:	IPS2302A
Serial Number:	504E005G2

Operating Modes

The EUT was tested in the following operating mode(s):

- Transmitting at maximum power with an 8 GHz chirp bandwidth and FMCW modulation.

Configuration and Peripherals


The EUT was tested in the following configuration(s):

- The EUT was configured using the built-in user interface. The chirp bandwidth was set by varying the maximum measurement distance setting.
- The EUT was powered via a 24 VDC bench power supply connected to a 120 VAC 60 Hz mains supply.
- Testing was performed with the EUT installed in a representative metal tank. No accessories/peripherals were employed during test as there were no ports on the EUT to populate.
- Testing was performed with the EUT transmitting an 8 GHz chirp bandwidth, as preliminary investigation showed this to be the worst case with respect to emissions.
- The EUT can be supplied with a range of antennas. Testing was performed on the highest gain antenna of each type.

Test Setup Diagrams


Radiated Tests:

Test Setup for Transmitter Radiated Emissions

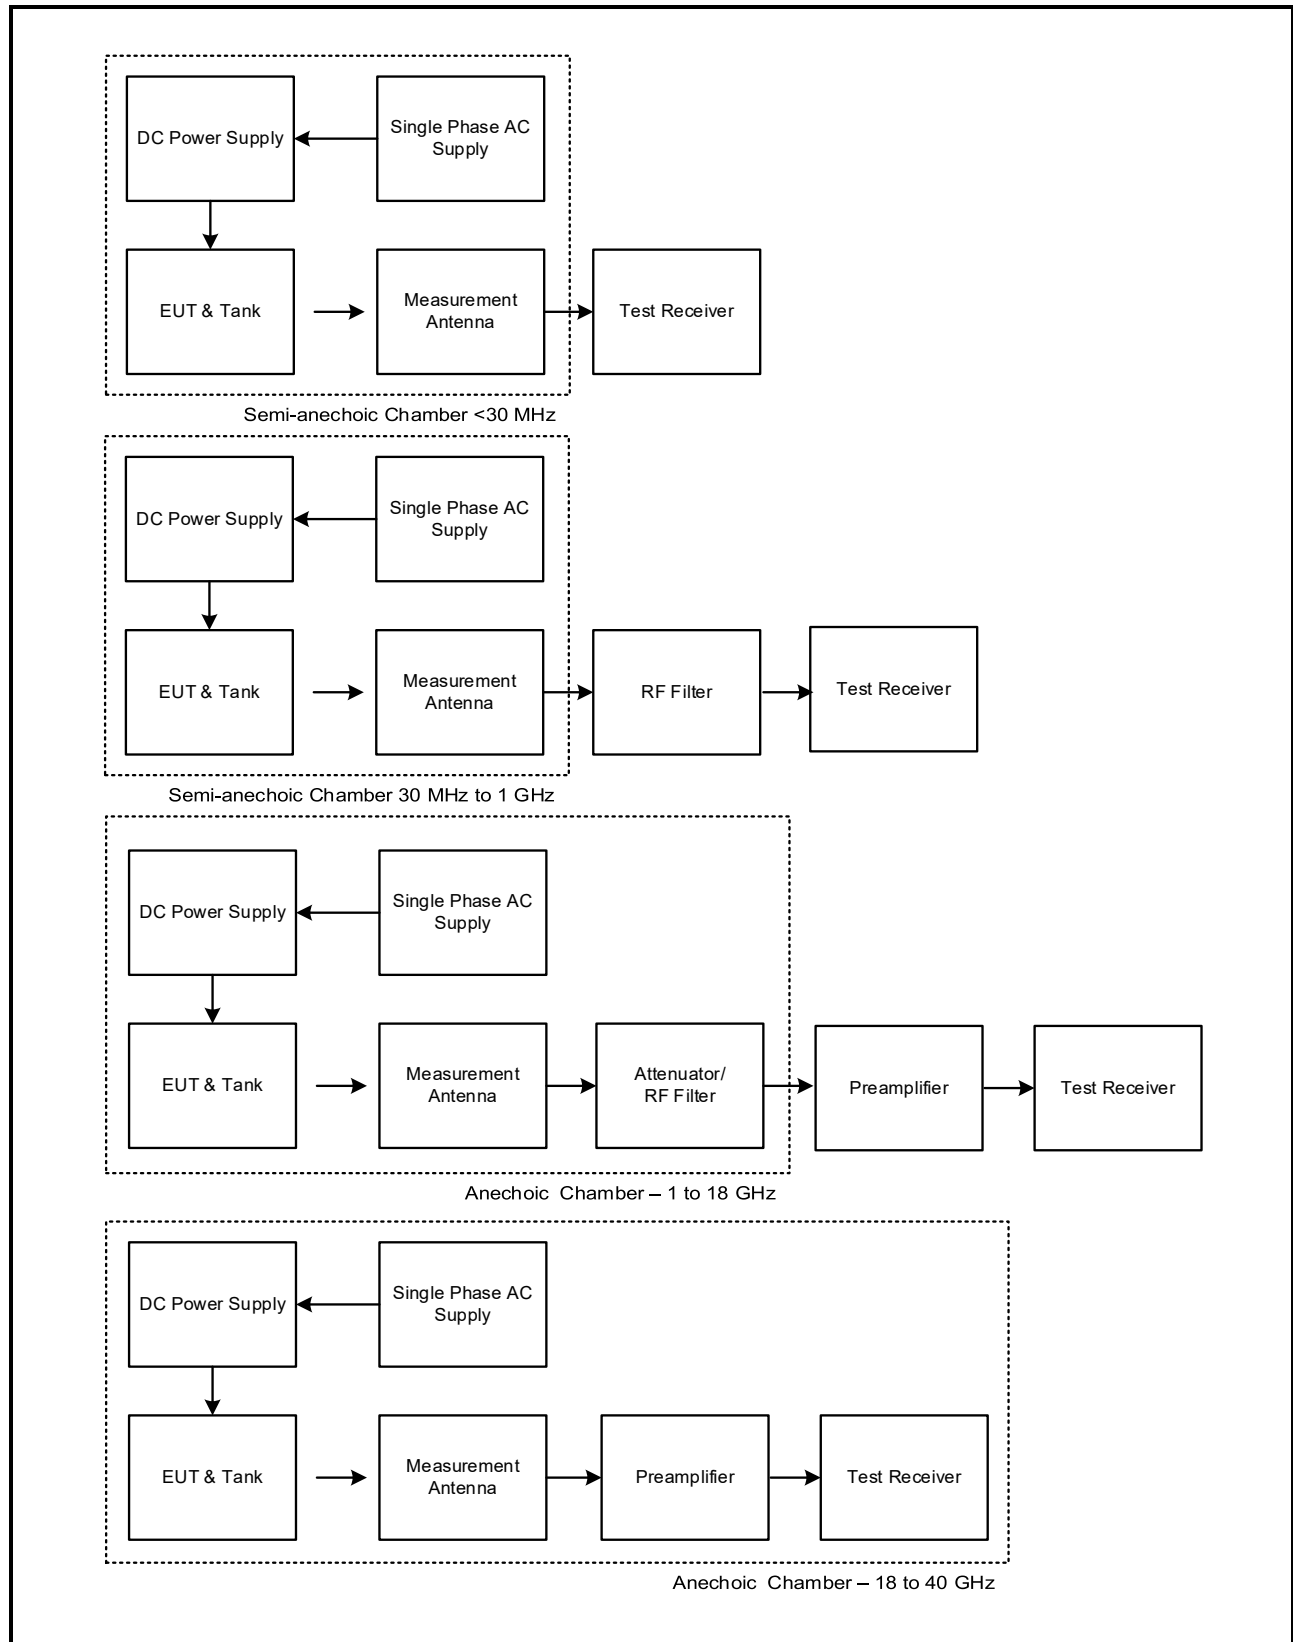


Test Setup Diagrams (continued)

Test Setup for Transmitter Radiated Emissions (continued)

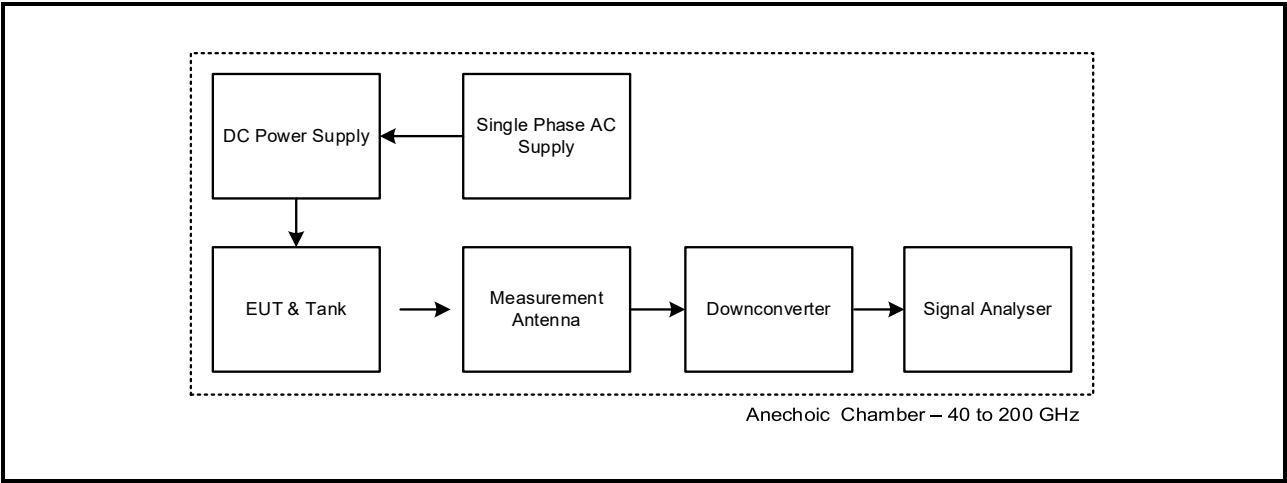

Test Setup for Transmitter AC Conducted Spurious Emissions

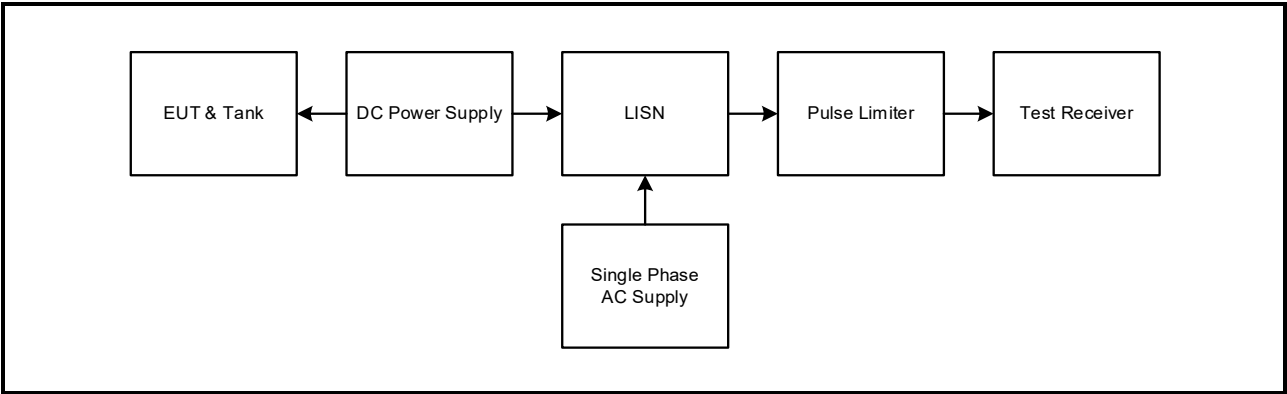

4 Radiated Test Results

4.1 Transmitter Radiated Emissions <1 GHz

Test Summary:

Test Engineer:	Mark Perry	Test Dates:	15 August 2021 & 02 October 2021
Test Sample Serial Number:	52403535		

FCC Reference:	Part 15.31(q) & 15.209(a)
Test Method Used:	ANSI C63.10 Sections 6.3, 6.4 and 6.5
Frequency Range	9 kHz to 1000 MHz

Environmental Conditions:




Temperature (°C):	24 to 25
Relative Humidity (%):	41 to 46

Note(s):

1. The final measured value, for the given emission, in the table below incorporates the calibrated antenna factor and cable loss.
2. All other emissions shown on the pre-scans were investigated and found to be ambient, or > 20 dB below the appropriate limit or below the noise floor of the measurement system.
3. Measurements below 1 GHz were performed in semi-anechoic chambers (Asset Numbers K0001 & K0017) at a distance of 3 metres. The EUT was placed at a height of 80 cm above the reference ground plane in the centre of the chamber turntable. Between 30 MHz and 1 GHz, maximum emission levels were determined by height searching the measurement antenna over the range 1 metre to 4 metres.
4. Pre-scans were performed and markers placed on the highest measured levels. The test receiver was configured as follows: For 9 kHz to 150 kHz, the resolution bandwidth was set to 300 Hz and video bandwidth 1 kHz. A peak detector was used and trace mode was Max Hold. For 150 kHz to 30 MHz, the resolution bandwidth was set to 10 kHz and video bandwidth 30 kHz, trace mode was Max Hold. For 30 MHz to 1 GHz, the resolution bandwidth was set to 120 kHz and video bandwidth 500 kHz. A peak detector was used, sweep time was set to auto and trace mode was Max Hold.
5. Pre-scans were performed with each antenna. Emission frequencies and amplitudes did not vary between antennas, therefore final measurements were performed on the Plastic Horn Antenna.
6. Final measurements were performed on the marker frequencies and the results entered into the table below. The test receiver resolution bandwidth was set to 120 kHz, using a CISPR quasi-peak detector and span wide enough to see the whole emission.

Transmitter Radiated Emissions (continued)**Results: Quasi-Peak**

Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
46.355	Vertical	23.0	40.0	17.0	Complied
57.225	Vertical	31.4	40.0	8.6	Complied
62.550	Vertical	25.0	40.0	15.0	Complied

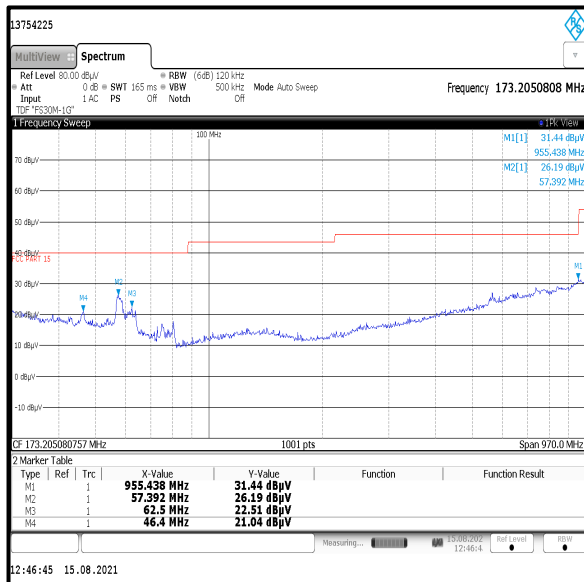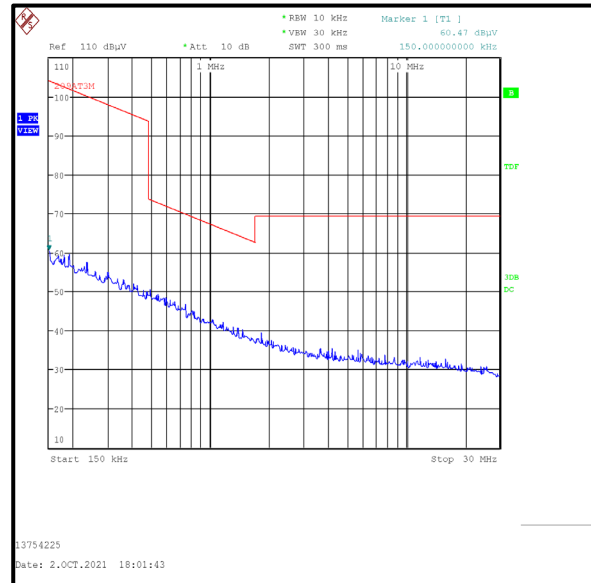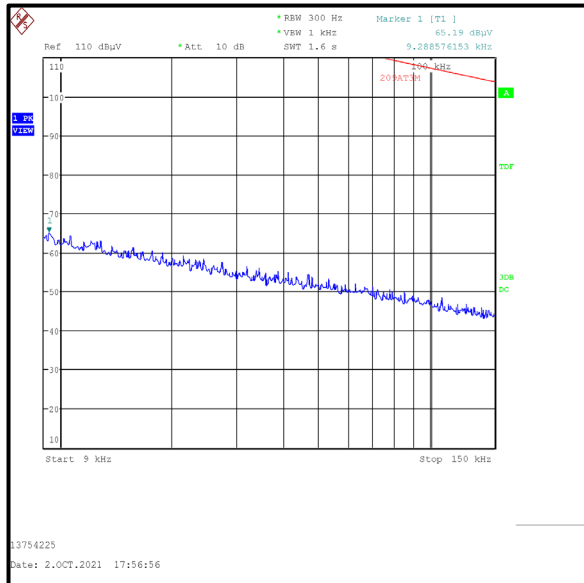

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying table.

4.2 Transmitter Radiated Emissions >1 GHz

Test Summary:

Test Engineers:	Mark Perry, Vi Van, Saurabh Bhandari & Ben Mercer	Test Dates:	14 August 2021 to 25 September 2021
Test Sample Serial Number:	52403535		

FCC Reference:	Part 15.31(q) & 15.209(a)
Test Method Used:	ANSI C63.10 Sections 6.3, 6.6, 9.8 and 9.12
Frequency Range	1 GHz to 200 GHz

Environmental Conditions:

Temperature (°C):	24 to 25
Relative Humidity (%):	41 to 58

Note(s):

1. The final measured value, for the given emission, in the table below incorporates the calibrated antenna factor and cable loss.
2. All other emissions shown on the pre-scans were investigated and found to be ambient, or > 20 dB below the appropriate limit or below the noise floor of the measurement system. Where no emissions < 20 dB from the applicable limit were identified, the highest noise floor reading was reported in the tables below.
3. Pre-scans above 1 GHz were performed in fully anechoic chambers (Asset Numbers K0002 & K0017) at a distance of 3 metres. The EUT was placed at a height of 1.5 metres above the test chamber floor in the centre of the chamber turntable. All measurement antennas were placed at a fixed height of 1.5 metres above the test chamber floor, in line with the EUT.
4. Final measurements between 1 GHz and 40 GHz were performed in a fully anechoic chamber (Asset Number K0017) at a distance of 3 metres. The EUT was placed at a height of 1.5 m above the reference ground plane in the centre of the chamber turntable. Maximum emission levels were determined by height searching the measurement antenna over the range 1 metre to 4 metres.
5. Measurements above 40 GHz were performed in accordance with ANSI C63.10 Clause 9.12.
6. Measurement distances above 40 GHz were determined according to ANSI C63.10 Clause 9.8. Measurement distances were reduced until 6 dB noise floor clearance was achieved:





40-50 GHz – 0.05 metres
50-75 GHz – 0.2 metres
75-110 GHz – 0.1 metres
110-170 GHz – 0.2 metres
170-200 GHz – 0.2 metres
7. Pre-scans were performed up to 210 GHz, results are valid up to 200 GHz.

Transmitter Radiated Emissions (continued)**Results: VEGAZW-6-74537 / Peak**




Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
81610.000	Horizontal	64.9	74.0	9.1	Complied

Results: VEGAZW-6-74537 / Average

Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
81610.000	Horizontal	31.2	54.0	22.8	Complied

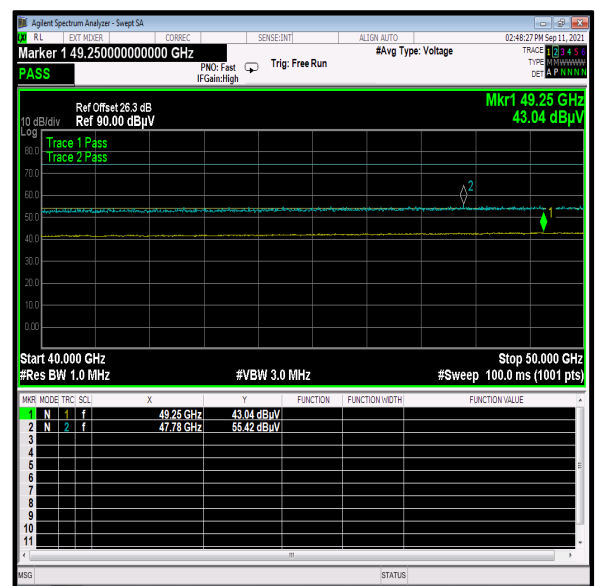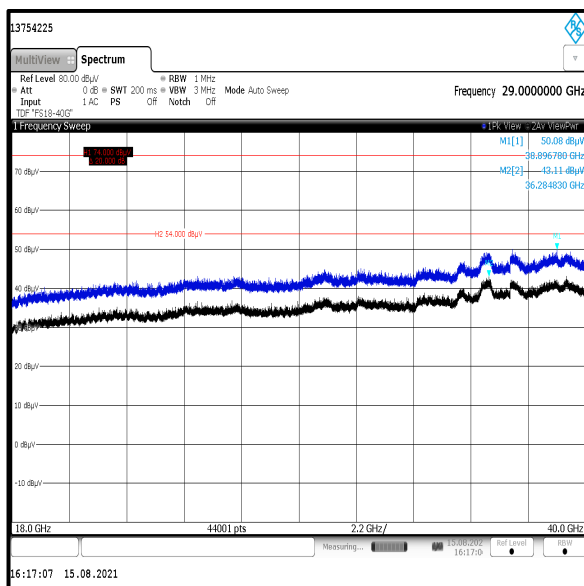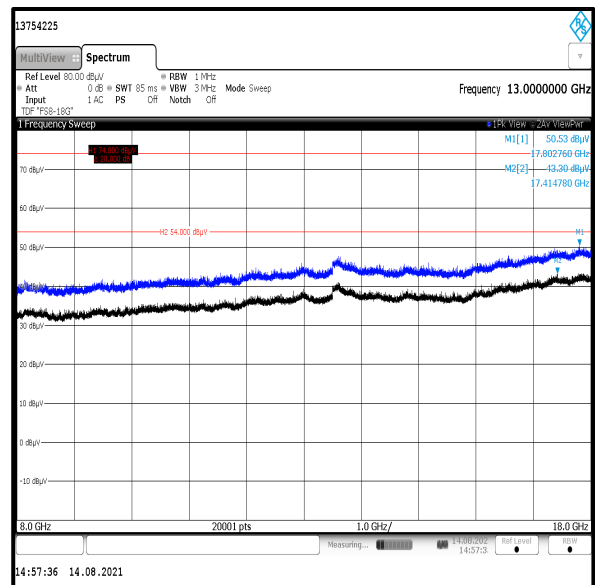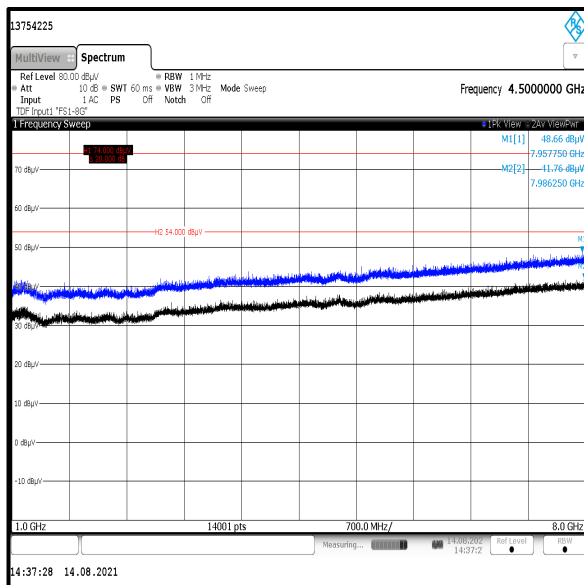

Note: The above plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

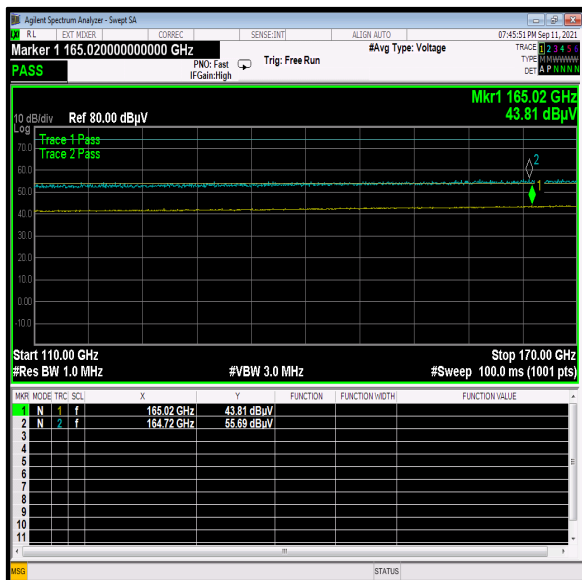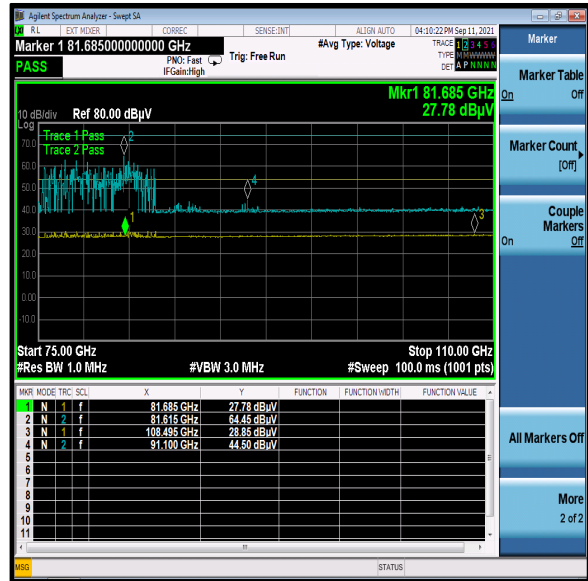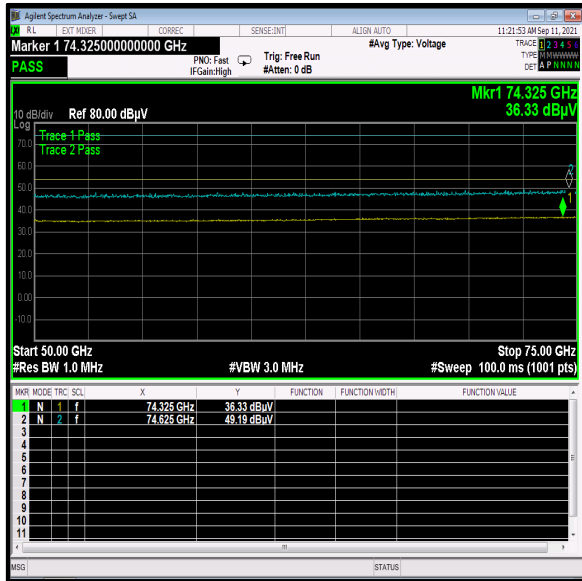Transmitter Radiated Emissions (continued)

Note: The above plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.




Transmitter Radiated Emissions (continued)

Results: VEGAZW-6-74539 / Peak





Frequency (MHz)	Antenna Polarity	Level (dBμV/m)	Limit (dBμV/m)	Margin (dB)	Result
200000.000	Horizontal	57.5	74.0	16.5	Complied

Results: VEGAZW-6-74539 / Average

Frequency (MHz)	Antenna Polarity	Level (dBμV/m)	Limit (dBμV/m)	Margin (dB)	Result
199200.000	Horizontal	44.8	54.0	9.2	Complied

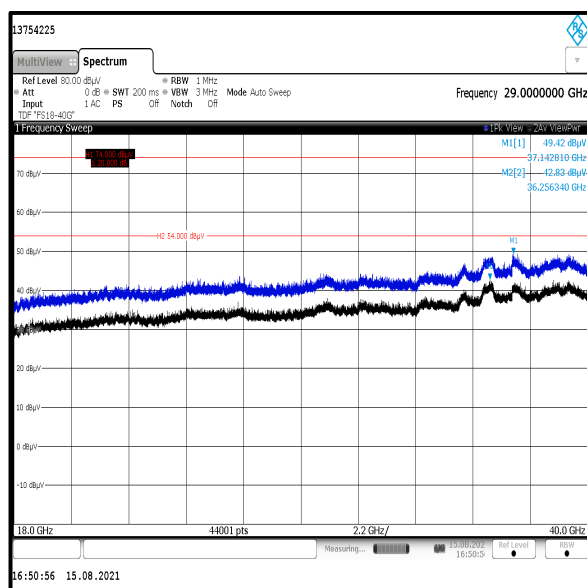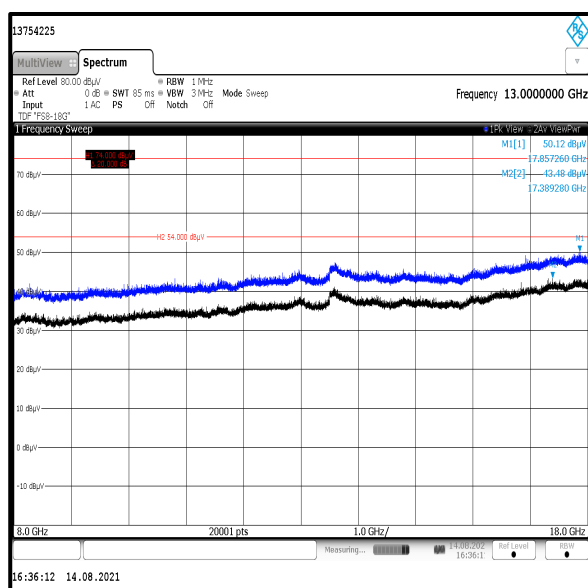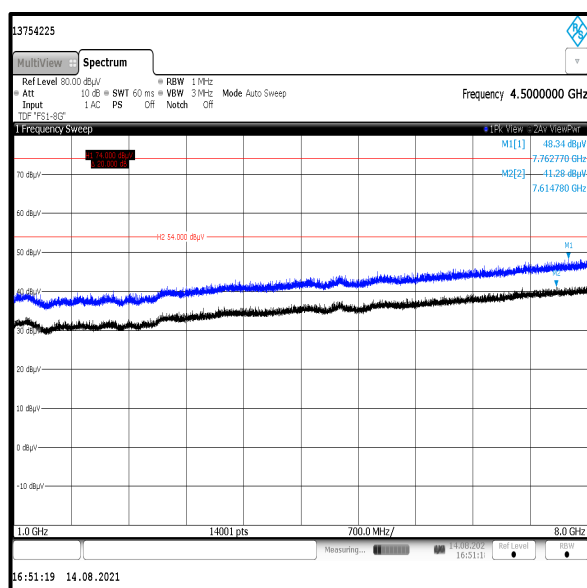

Transmitter Radiated Emissions (continued)

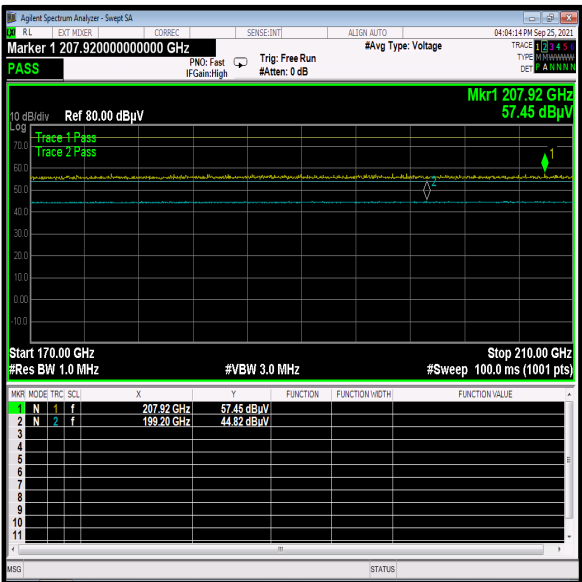
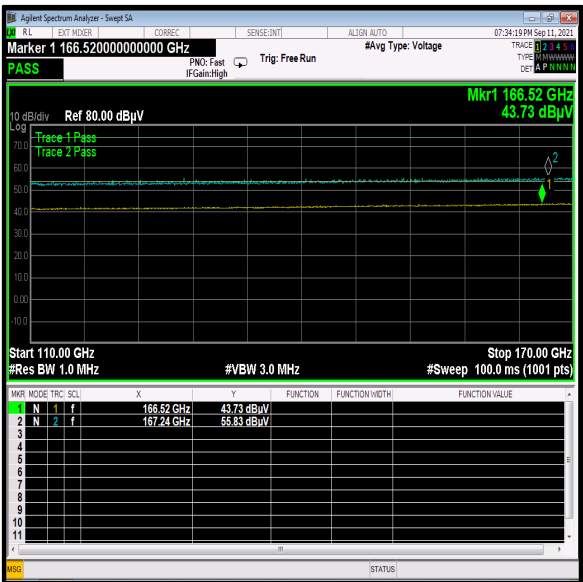
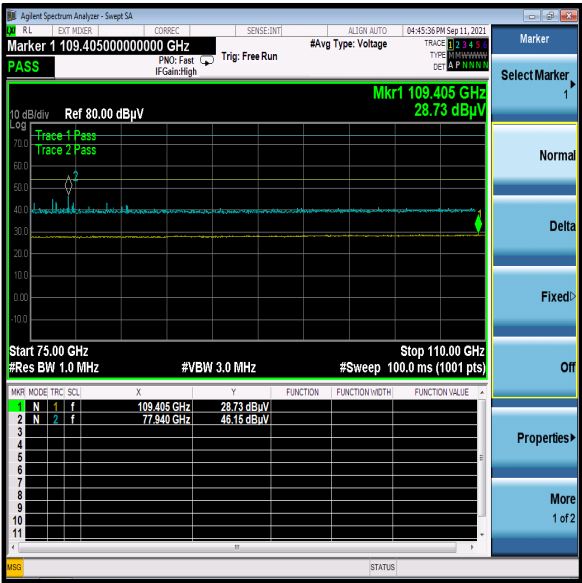
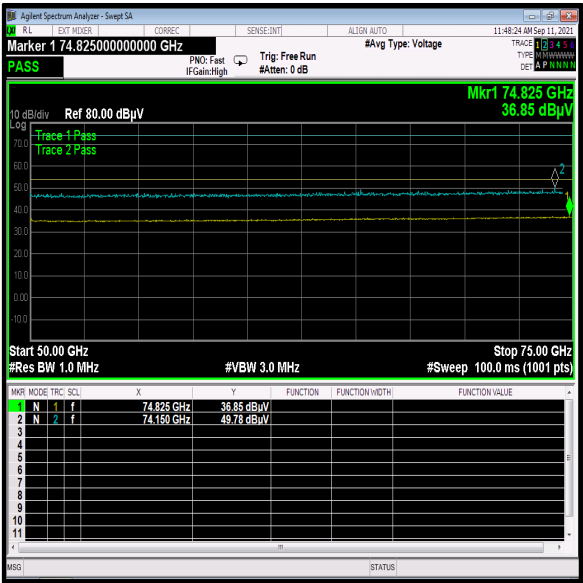


Transmitter Radiated Emissions (continued)**Results: VEGAZW-6-74547 / Peak**



Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
79375.000	Horizontal	66.8	74.0	7.2	Complied

Results: VEGAZW-6-74547 / Average

Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
79375.000	Horizontal	32.1	54.0	21.9	Complied

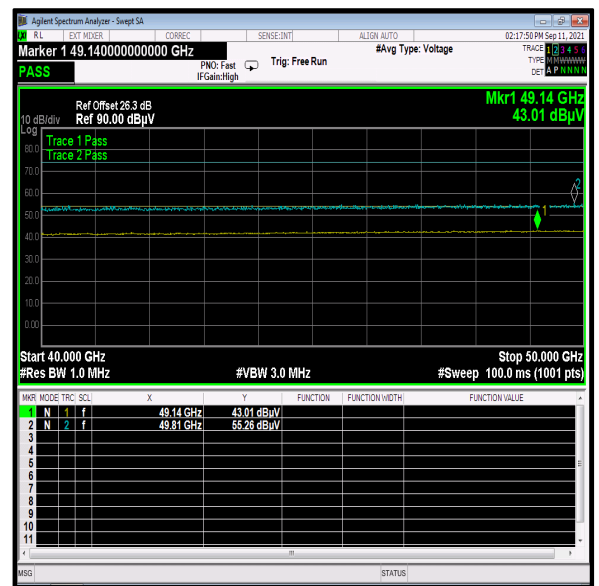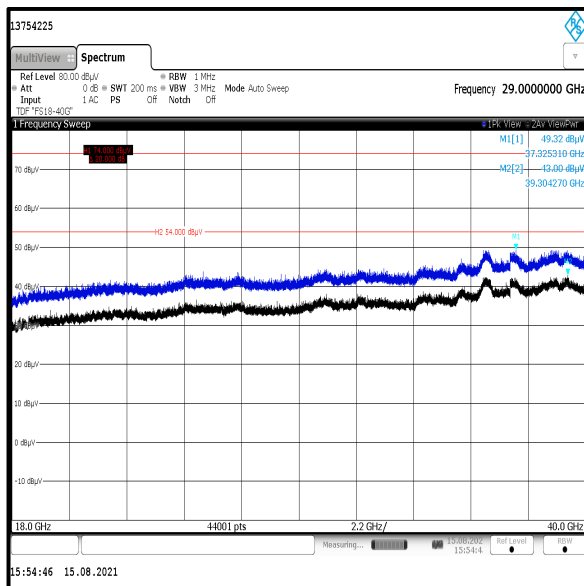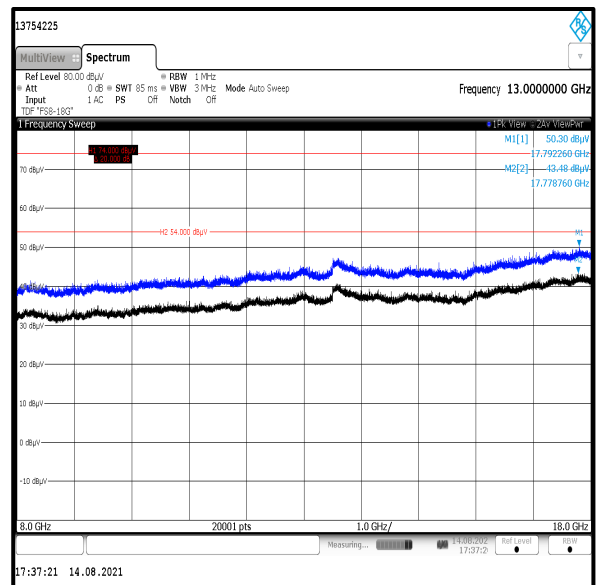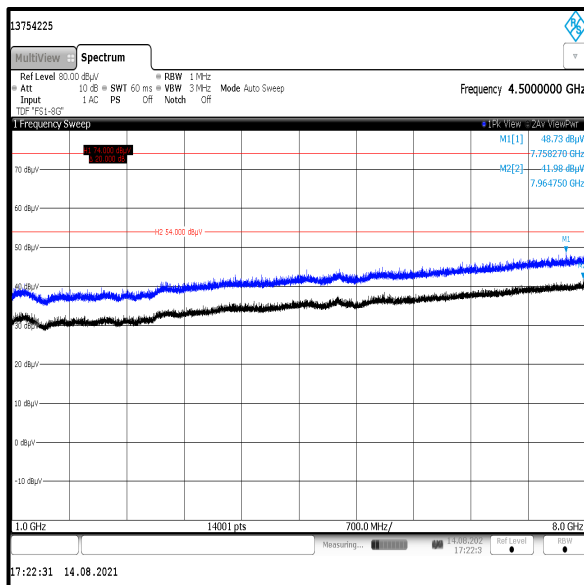

Note: The above plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

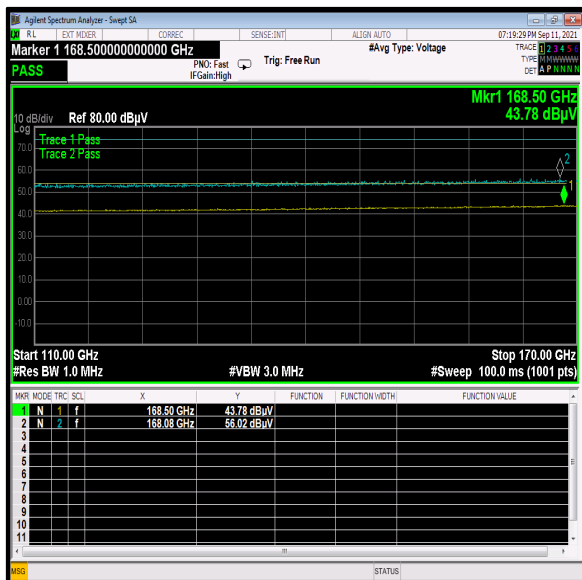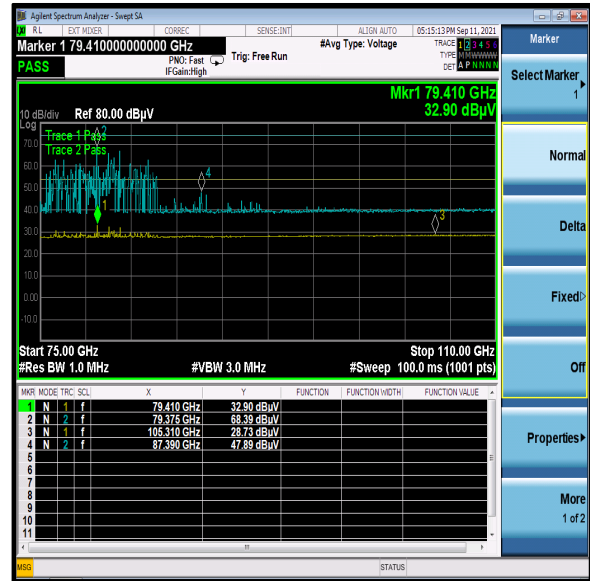Transmitter Radiated Emissions (continued)





Note: The above plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.





Transmitter Radiated Emissions (continued)**Results: VEGAZW-6-74538 / Peak**

Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
189360.000	Horizontal	58.3	74.0	15.7	Complied

Results: VEGAZW-6-74538 / Average

Frequency (MHz)	Antenna Polarity	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Result
173600.000	Horizontal	44.8	54.0	9.2	Complied

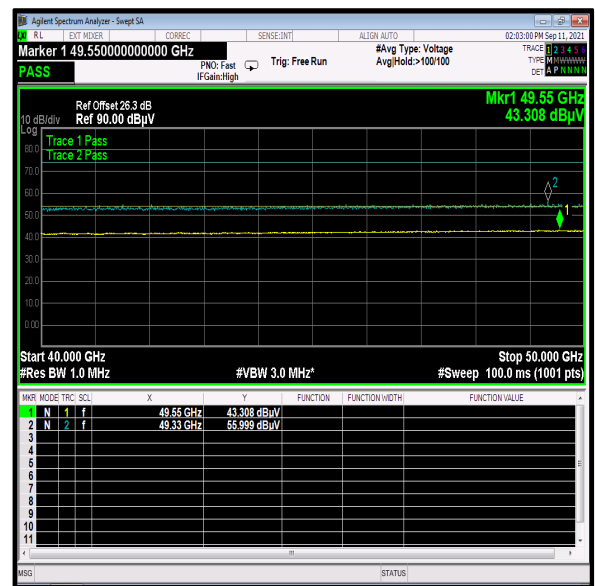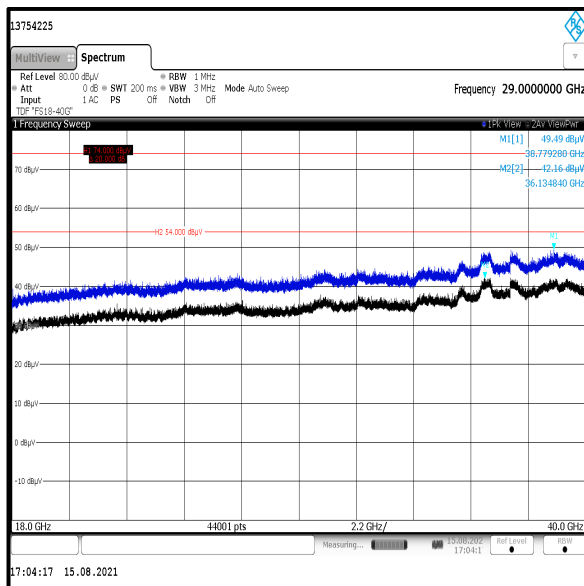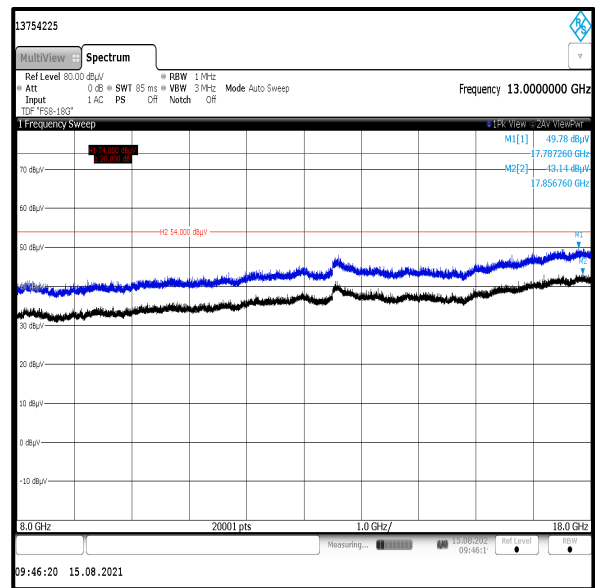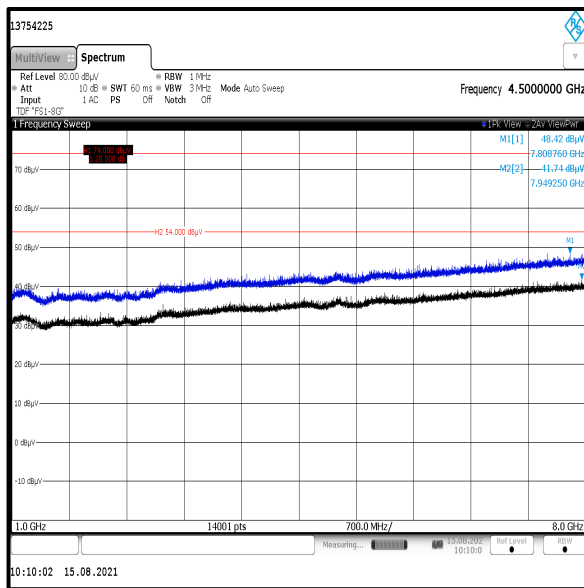

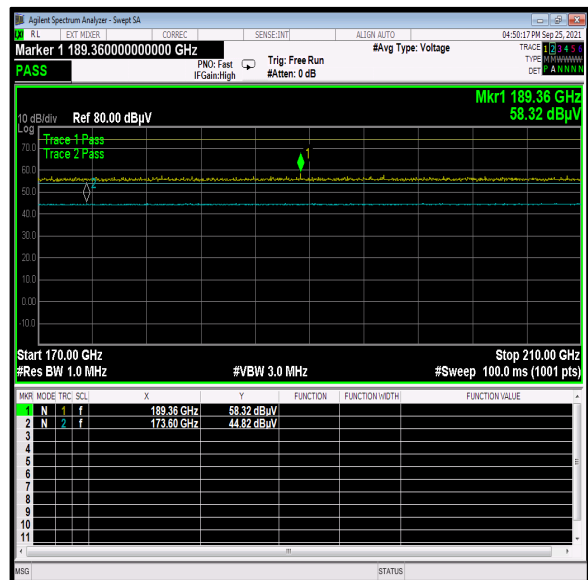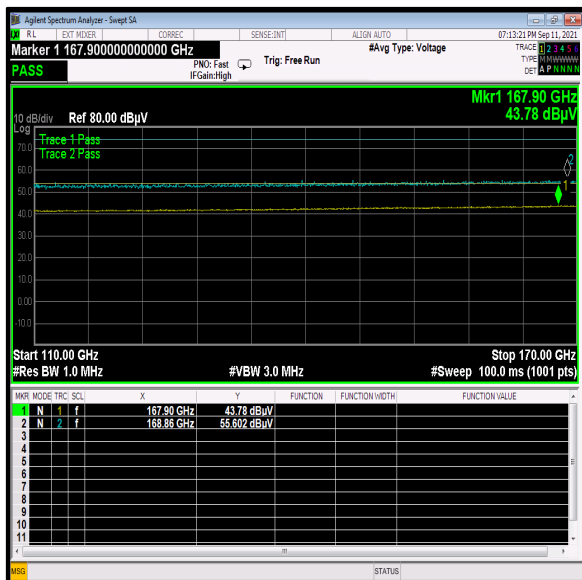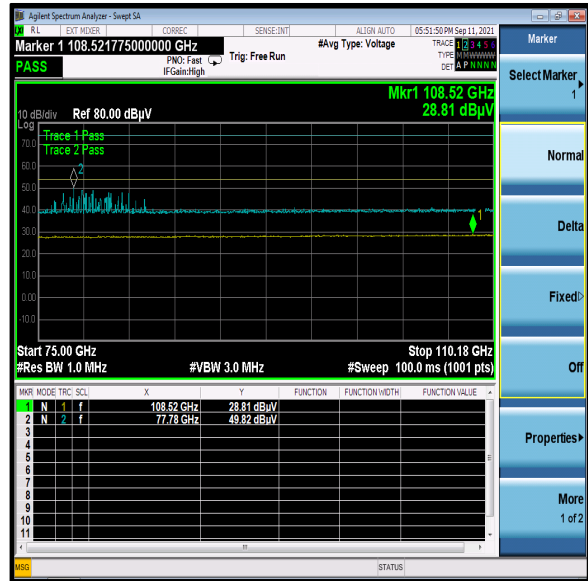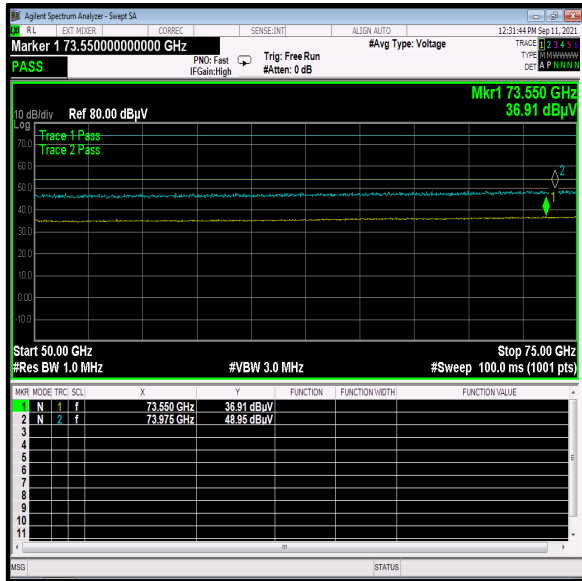Transmitter Radiated Emissions (continued)

5 AC Power Line Conducted Emissions Test Results

5.1 Transmitter AC Conducted Spurious Emissions

Test Summary:

Test Engineers:	Alison Johnston & Nick Raptopoulos	Test Dates:	04 October 2021 & 05 October 2021
Test Sample Serial Number:	52403535		

FCC Reference:	Part 15.207
Test Method Used:	ANSI C63.10 Section 6.2 / FCC KDB 174176 and notes below

Environmental Conditions:

Temperature (°C):	22
Relative Humidity (%):	60

Note(s):

1. The EUT was connected to a 24 VDC bench power supply. The DC power supply was connected to 120 VAC 60 Hz single phase supply via a LISN.
2. In accordance with FCC KDB 174176 Q4, tests were performed with a 240 VAC 60 Hz single phase supply as this was within the voltage range marked on the power supply.
3. A pulse limiter was fitted between the LISN and the test receiver.
4. Pre-scans were performed and markers placed on the highest live and neutral measured levels. Final measurements were performed on the marker frequencies and the results entered into the tables below.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74537 / Live / Quasi Peak / 120 VAC 60 Hz**

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.159	Live	36.7	65.5	28.8	Complied
0.281	Live	21.4	60.8	39.4	Complied
3.561	Live	13.3	56.0	42.7	Complied
6.387	Live	17.5	60.0	42.5	Complied
12.003	Live	11.0	60.0	49.0	Complied
16.395	Live	20.5	60.0	39.5	Complied

Results: VEGAZW-6-74537 / Live / Average / 120 VAC 60 Hz

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.164	Live	15.9	55.3	39.4	Complied
0.254	Live	14.0	51.6	37.6	Complied
1.532	Live	8.0	46.0	38.0	Complied
11.999	Live	5.0	50.0	45.0	Complied
13.560	Live	42.0	50.0	8.0	Complied
16.229	Live	19.7	50.0	30.3	Complied

Results: VEGAZW-6-74537 / Neutral / Quasi Peak / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.168	Neutral	35.3	65.1	29.8	Complied
0.285	Neutral	20.5	60.7	40.2	Complied
4.547	Neutral	14.6	56.0	41.4	Complied
6.252	Neutral	16.6	60.0	43.4	Complied
12.003	Neutral	10.9	60.0	49.1	Complied
16.319	Neutral	20.7	60.0	39.3	Complied

Results: VEGAZW-6-74537 / Neutral / Average / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.164	Neutral	15.7	55.3	39.6	Complied
0.267	Neutral	13.3	51.2	37.9	Complied
1.518	Neutral	8.0	46.0	38.0	Complied
6.450	Neutral	5.6	50.0	44.4	Complied
11.994	Neutral	4.9	50.0	45.1	Complied
16.233	Neutral	13.8	50.0	36.2	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74537 / 120 VAC 60 Hz

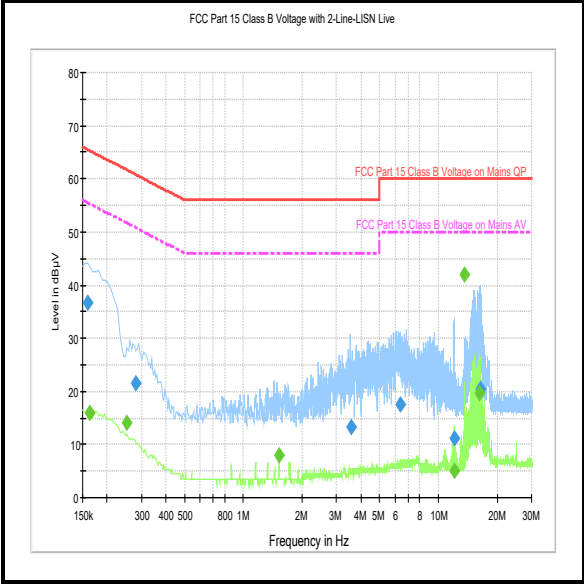

Live

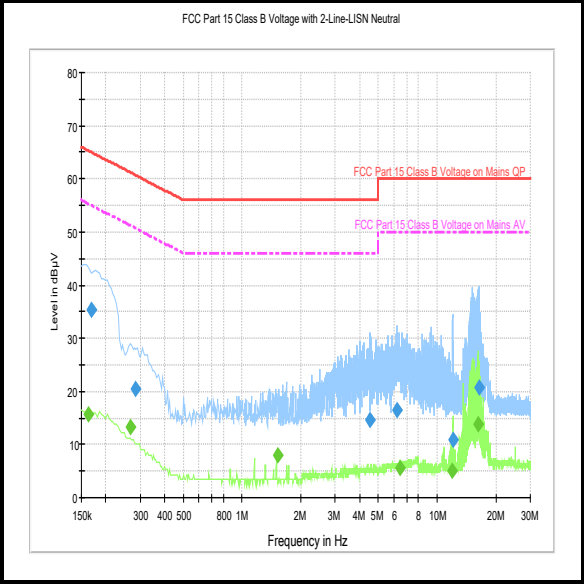

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74537 / Live / Quasi Peak / 240 VAC 60 Hz**

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.177	Live	22.3	64.6	42.3	Complied
1.518	Live	8.0	56.0	48.0	Complied
6.801	Live	16.0	60.0	44.0	Complied
11.999	Live	11.0	60.0	49.0	Complied
16.229	Live	24.3	60.0	35.7	Complied
28.275	Live	10.4	60.0	49.6	Complied

Results: VEGAZW-6-74537 / Live / Average / 240 VAC 60 Hz

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.182	Live	13.5	54.4	40.9	Complied
1.532	Live	12.1	46.0	33.9	Complied
11.999	Live	5.9	50.0	44.1	Complied
13.560	Live	19.2	50.0	30.8	Complied
16.175	Live	10.8	50.0	39.2	Complied
25.058	Live	16.1	50.0	33.9	Complied

Results: VEGAZW-6-74537 / Neutral / Quasi Peak / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.191	Neutral	20.8	64.0	43.2	Complied
3.345	Neutral	13.3	56.0	42.7	Complied
6.315	Neutral	17.4	60.0	42.6	Complied
11.999	Neutral	13.2	60.0	46.8	Complied
16.454	Neutral	20.1	60.0	39.9	Complied
24.257	Neutral	10.5	60.0	49.5	Complied

Results: VEGAZW-6-74537 / Neutral / Average / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.200	Neutral	13.5	53.6	40.1	Complied
0.330	Neutral	11.2	49.5	38.3	Complied
1.338	Neutral	4.5	46.0	41.5	Complied
11.999	Neutral	7.2	50.0	42.8	Complied
15.464	Neutral	13.0	50.0	37.0	Complied
25.058	Neutral	23.5	50.0	26.5	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74537 / 240 VAC 60 Hz

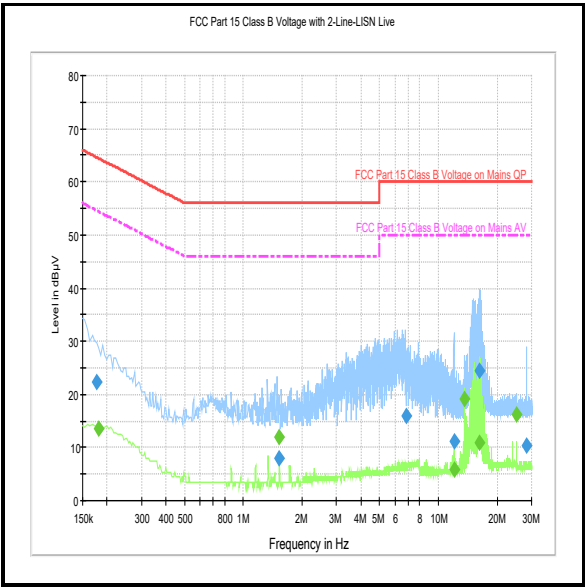

Live

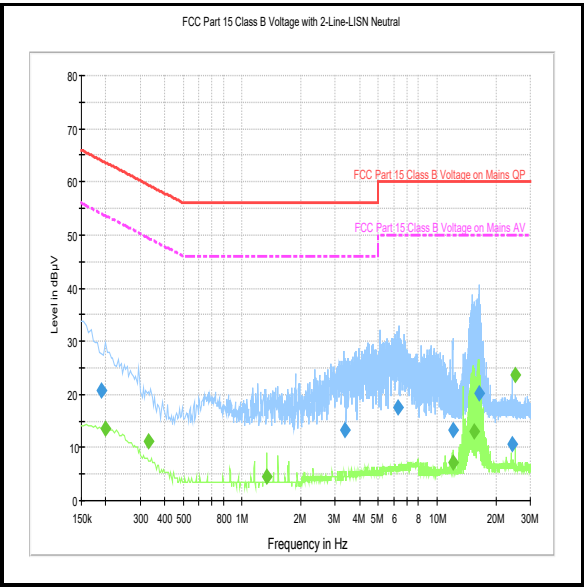

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74539 / Live / Quasi Peak / 120 VAC 60 Hz**

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.159	Live	36.9	65.5	28.6	Complied
4.088	Live	13.9	56.0	42.1	Complied
6.936	Live	15.5	60.0	44.5	Complied
11.999	Live	11.0	60.0	49.0	Complied
16.382	Live	20.8	60.0	39.2	Complied
22.349	Live	10.7	60.0	49.3	Complied

Results: VEGAZW-6-74539 / Live / Average / 120 VAC 60 Hz

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.200	Live	16.8	53.6	36.8	Complied
1.536	Live	7.4	46.0	38.6	Complied
7.967	Live	6.4	50.0	43.6	Complied
11.994	Live	5.0	50.0	45.0	Complied
16.391	Live	11.3	50.0	38.7	Complied
25.058	Live	12.2	50.0	37.8	Complied

Results: VEGAZW-6-74539 / Neutral / Quasi Peak / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.168	Neutral	36.6	65.1	28.5	Complied
0.299	Neutral	20.8	60.3	39.5	Complied
3.494	Neutral	12.9	56.0	43.1	Complied
5.928	Neutral	15.3	60.0	44.7	Complied
11.999	Neutral	12.2	60.0	47.8	Complied
16.395	Neutral	20.1	60.0	39.9	Complied

Results: VEGAZW-6-74539 / Neutral / Average / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.200	Neutral	16.6	53.6	37.0	Complied
0.335	Neutral	13.3	49.3	36.0	Complied
11.999	Neutral	6.5	50.0	43.5	Complied
14.595	Neutral	12.7	50.0	37.3	Complied
16.391	Neutral	12.0	50.0	38.0	Complied
25.058	Neutral	16.1	50.0	33.9	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74539 / 120 VAC 60 Hz

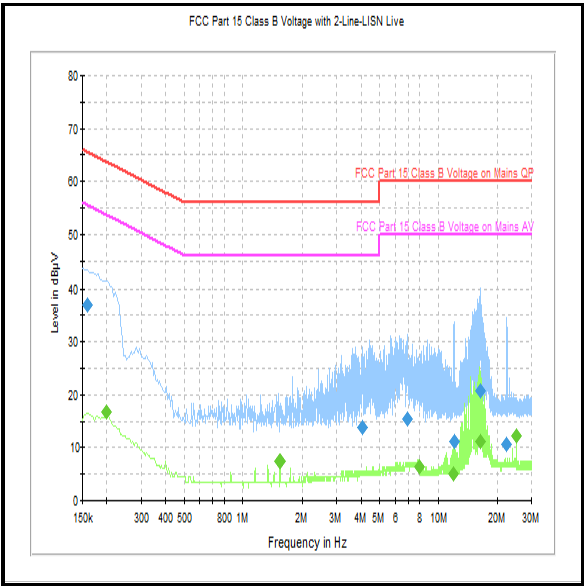

Live

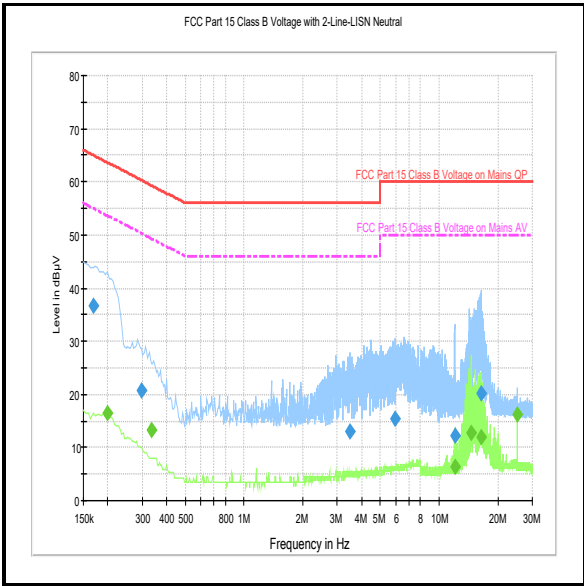

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74539 / Live / Quasi Peak / 240 VAC 60 Hz**

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.182	Live	21.6	64.4	42.8	Complied
4.029	Live	14.5	56.0	41.5	Complied
6.468	Live	17.3	60.0	42.7	Complied
11.999	Live	14.0	60.0	46.0	Complied
16.364	Live	20.1	60.0	39.9	Complied
25.058	Live	25.1	60.0	34.9	Complied

Results: VEGAZW-6-74539 / Live / Average / 240 VAC 60 Hz

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.200	Live	14.6	53.6	39.0	Complied
0.335	Live	11.6	49.3	37.7	Complied
4.551	Live	4.7	46.0	41.3	Complied
11.967	Live	6.6	50.0	43.4	Complied
14.316	Live	27.9	50.0	22.1	Complied
25.058	Live	24.6	50.0	25.4	Complied

Results: VEGAZW-6-74539 / Neutral / Quasi Peak / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.168	Neutral	23.9	65.1	41.2	Complied
2.616	Neutral	10.6	56.0	45.4	Complied
6.252	Neutral	17.2	60.0	42.8	Complied
11.999	Neutral	13.9	60.0	46.1	Complied
16.391	Neutral	19.5	60.0	40.5	Complied
25.058	Neutral	25.3	60.0	34.7	Complied

Results: VEGAZW-6-74539 / Neutral / Average / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.200	Neutral	14.6	53.6	39.0	Complied
2.6566	Neutral	5.5	46.0	40.5	Complied
6.450	Neutral	6.3	50.0	43.7	Complied
11.967	Neutral	7.2	50.0	42.8	Complied
16.305	Neutral	10.7	50.0	39.3	Complied
25.058	Neutral	24.5	50.0	25.5	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74539 / 240 VAC 60 Hz

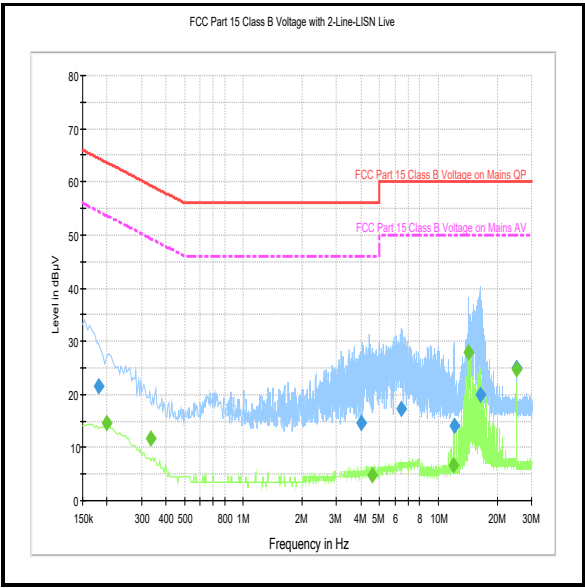

Live

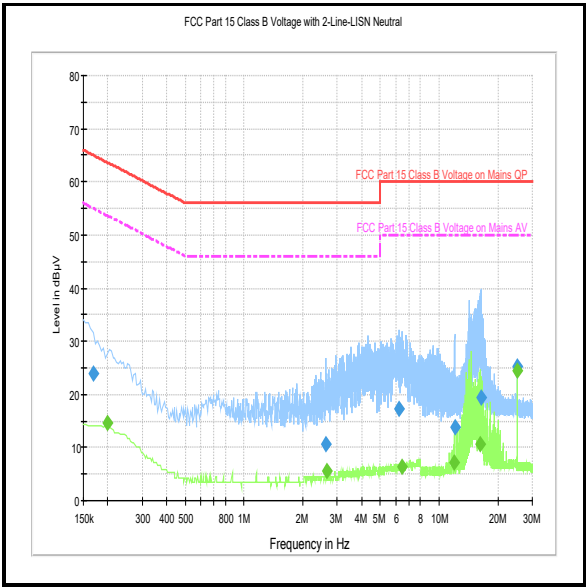

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74547 / Live / Quasi Peak / 120 VAC 60 Hz**

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.155	Live	38.5	65.8	27.3	Complied
0.29	Live	22.4	60.7	38.3	Complied
4.120	Live	14.5	56.0	41.5	Complied
6.509	Live	16.7	60.0	43.3	Complied
11.999	Live	14.0	60.0	46.0	Complied
16.395	Live	19.9	60.0	40.1	Complied

Results: VEGAZW-6-74547 / Live / Average / 120 VAC 60 Hz

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.173	Live	16.2	54.8	38.6	Complied
0.285	Live	10.0	50.7	40.7	Complied
11.999	Live	8.5	50.0	41.5	Complied
16.179	Live	10.8	50.0	39.2	Complied
18.011	Live	12.2	50.0	37.8	Complied
25.058	Live	18.0	50.0	32.0	Complied

Results: VEGAZW-6-74547 / Neutral / Quasi Peak / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.173	Neutral	37.3	64.8	27.5	Complied
4.263	Neutral	15.1	56.0	40.9	Complied
6.666	Neutral	16.6	60.0	43.4	Complied
11.999	Neutral	15.8	60.0	44.2	Complied
14.316	Neutral	34.9	60.0	25.1	Complied
21.359	Neutral	10.4	60.0	49.6	Complied

Results: VEGAZW-6-74547 / Neutral / Average / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.173	Neutral	16.2	54.8	38.6	Complied
0.285	Neutral	13.3	50.7	37.4	Complied
9.555	Neutral	4.9	50.0	45.1	Complied
12.003	Neutral	8.4	50.0	41.6	Complied
14.532	Neutral	19.4	50.0	30.6	Complied
25.058	Neutral	9.5	50.0	40.5	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74547 / 120 VAC 60 Hz

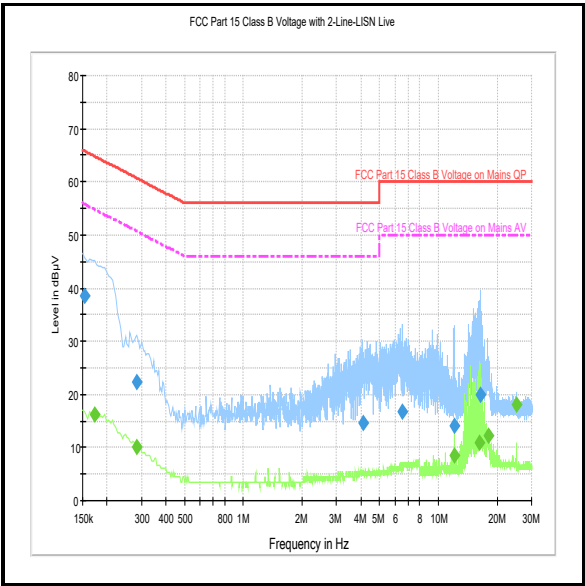

Live

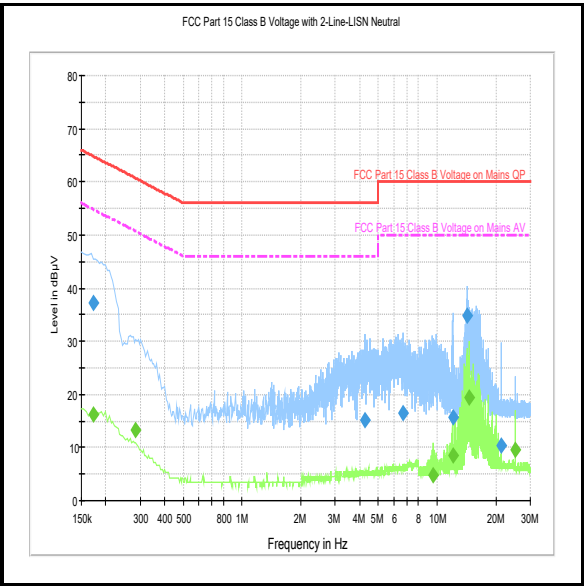

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74547 / Live / Quasi Peak / 240 VAC 60 Hz**

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.191	Live	26.4	64.0	37.6	Complied
0.942	Live	8.0	56.0	48.0	Complied
3.957	Live	14.8	56.0	41.2	Complied
6.059	Live	17.7	60.0	42.3	Complied
11.999	Live	11.0	60.0	49.0	Complied
16.458	Live	16.9	60.0	43.1	Complied

Results: VEGAZW-6-74547 / Live / Average / 240 VAC 60 Hz

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.168	Live	14.4	55.1	40.7	Complied
1.343	Live	11.3	46.0	34.7	Complied
3.876	Live	4.7	46.0	41.3	Complied
11.994	Live	5.0	50.0	45.0	Complied
16.449	Live	8.8	50.0	41.2	Complied
25.058	Live	12.2	50.0	37.8	Complied

Results: VEGAZW-6-74547 / Neutral / Quasi Peak / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.191	Neutral	25.8	64.0	38.2	Complied
2.949	Neutral	12.6	56.0	43.4	Complied
6.216	Neutral	17.2	60.0	42.8	Complied
12.003	Neutral	11.4	60.0	48.6	Complied
16.382	Neutral	18.4	60.0	41.6	Complied
21.822	Neutral	10.4	60.0	49.6	Complied

Results: VEGAZW-6-74547 / Neutral / Average / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.173	Neutral	14.4	54.8	40.4	Complied
0.281	Neutral	11.6	50.8	39.2	Complied
1.338	Neutral	6.8	46.0	39.2	Complied
11.994	Neutral	4.9	50.0	45.1	Complied
16.121	Neutral	9.2	50.0	40.8	Complied
25.058	Neutral	11.9	50.0	38.1	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74547 / 240 VAC 60 Hz

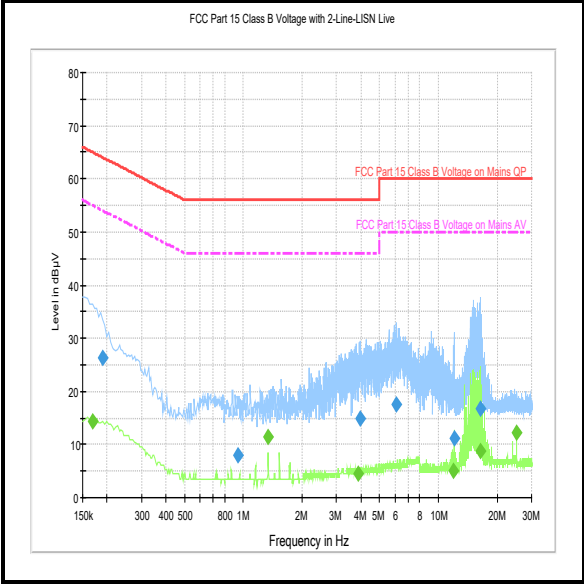

Live

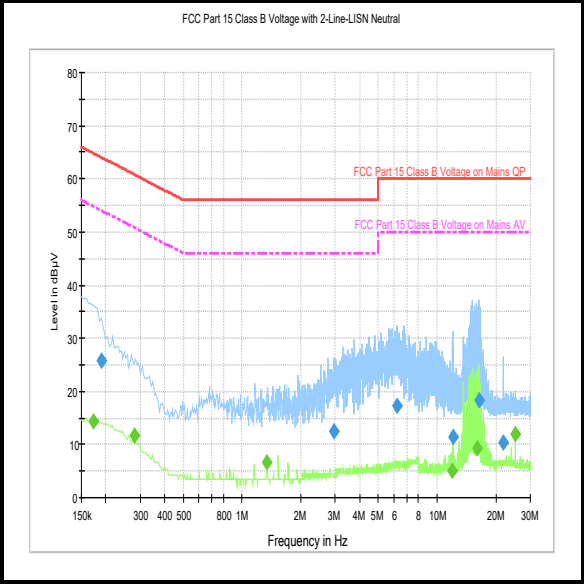

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74538 / Live / Quasi Peak / 120 VAC 60 Hz**

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.173	Live	37.1	64.8	27.7	Complied
0.299	Live	21.8	60.3	38.5	Complied
2.517	Live	11.0	56.0	45.0	Complied
6.171	Live	17.7	60.0	42.3	Complied
11.999	Live	11.5	60.0	48.5	Complied
16.382	Live	22.2	60.0	37.8	Complied

Results: VEGAZW-6-74538 / Live / Average / 120 VAC 60 Hz

Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.177	Live	15.9	54.6	38.7	Complied
0.272	Live	10.8	51.1	40.3	Complied
1.532	Live	8.0	46.0	38.0	Complied
11.999	Live	5.9	50.0	44.1	Complied
16.229	Live	19.0	50.0	31.0	Complied
25.058	Live	12.6	50.0	37.4	Complied

Results: VEGAZW-6-74538 / Neutral / Quasi Peak / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.173	Neutral	36.9	64.8	27.9	Complied
0.272	Neutral	22.3	61.1	38.8	Complied
3.930	Neutral	14.8	56.0	41.2	Complied
6.639	Neutral	16.8	60.0	43.2	Complied
11.999	Neutral	11.4	60.0	48.6	Complied
16.382	Neutral	21.9	60.0	38.1	Complied

Results: VEGAZW-6-74538 / Neutral / Average / 120 VAC 60 Hz


Frequency (MHz)	Line	Level (dBμV)	Limit (dBμV)	Margin (dB)	Result
0.177	Neutral	15.9	54.6	38.7	Complied
0.290	Neutral	10.0	50.5	40.5	Complied
1.338	Neutral	6.1	46.0	39.9	Complied
11.999	Neutral	5.8	50.0	44.2	Complied
16.341	Neutral	10.7	50.0	39.3	Complied
25.058	Neutral	12.7	50.0	37.3	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74538 / 120 VAC 60 Hz

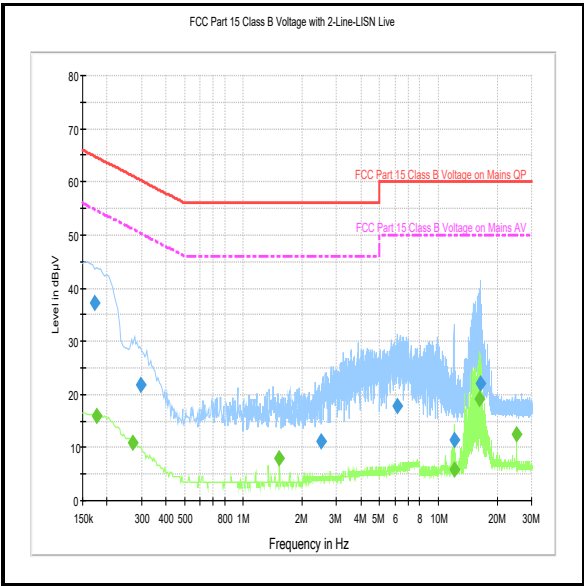

Live

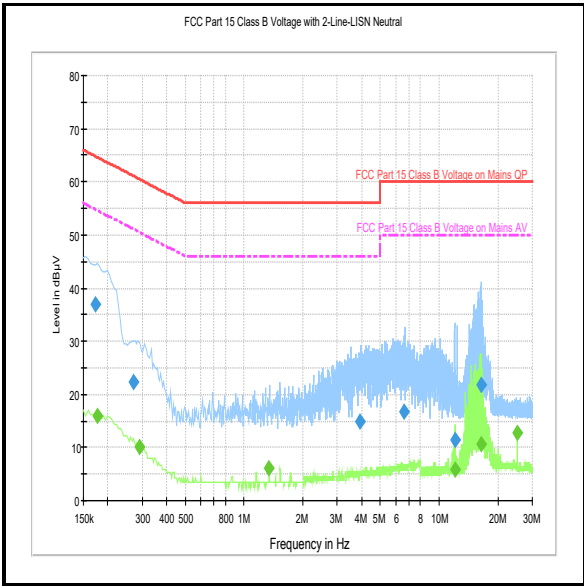

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

Transmitter AC Conducted Spurious Emissions (continued)**Results: VEGAZW-6-74538 / Live / Quasi Peak / 240 VAC 60 Hz**

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.196	Live	20.7	63.8	43.1	Complied
3.309	Live	12.9	56.0	43.1	Complied
6.707	Live	16.4	60.0	43.6	Complied
11.994	Live	11.9	60.0	48.1	Complied
16.386	Live	21.0	60.0	39.0	Complied
25.058	Live	24.3	60.0	35.7	Complied

Results: VEGAZW-6-74538 / Live / Average / 240 VAC 60 Hz

Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.204	Live	13.5	53.4	39.9	Complied
0.281	Live	11.6	50.8	39.2	Complied
3.386	Live	4.6	46.0	41.4	Complied
11.999	Live	6.6	50.0	43.4	Complied
16.445	Live	11.7	50.0	38.3	Complied
25.058	Live	23.6	50.0	26.4	Complied

Results: VEGAZW-6-74538 / Neutral / Quasi Peak / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.200	Neutral	20.5	63.6	43.1	Complied
0.672	Neutral	10.0	56.0	46.0	Complied
6.000	Neutral	17.0	60.0	43.0	Complied
10.014	Neutral	13.2	60.0	46.8	Complied
16.454	Neutral	20.8	60.0	39.2	Complied
25.058	Neutral	23.4	60.0	36.6	Complied

Results: VEGAZW-6-74538 / Neutral / Average / 240 VAC 60 Hz


Frequency (MHz)	Line	Level (dB μ V)	Limit (dB μ V)	Margin (dB)	Result
0.200	Neutral	13.8	53.6	39.8	Complied
0.456	Neutral	5.2	46.8	41.6	Complied
11.999	Neutral	5.8	50.0	44.2	Complied
16.233	Neutral	18.0	50.0	32.0	Complied
20.000	Neutral	12.4	50.0	37.6	Complied
25.058	Neutral	22.5	50.0	27.5	Complied

Transmitter AC Conducted Spurious Emissions (continued)

Results: VEGAZW-6-74538 / 240 VAC 60 Hz

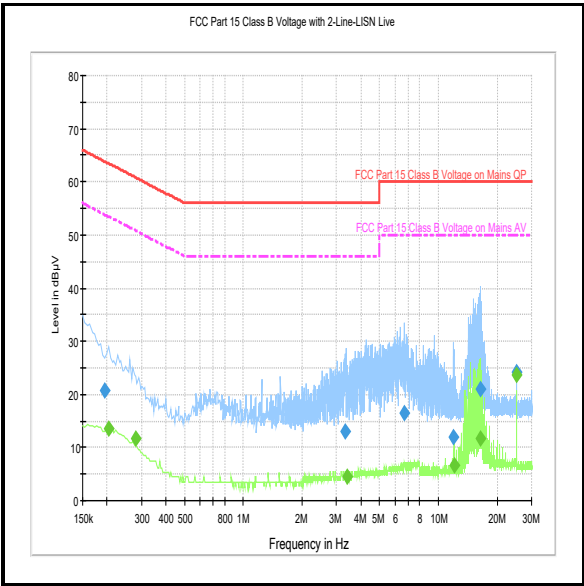

Live

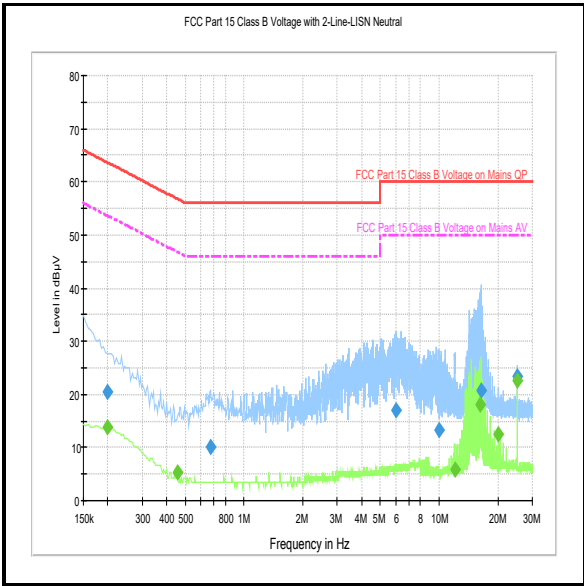

Neutral

Note: These plots are pre-scans and for indication purposes only. For final measurements, see accompanying tables.

--- END OF REPORT ---