Report No. : ES/2006/20002 Page : 1 of 26

Contents

APPENDIX


1. Photographs of Test Setup	02
2. Photographs of EUT	06
3. Photographs of the Battery	09
4. Photographs of the Accessories	11
5. Probe Calibration certificate	13
6. Uncertainty Analysis	21
7. Phantom description	22
8. System Validation from Original equipment supplier	23

Report No. : ES/2006/20002 Page : 2 of 26

Appendix Photographs of Test Setup




Fig.1 Photograph of the SAR measurement System

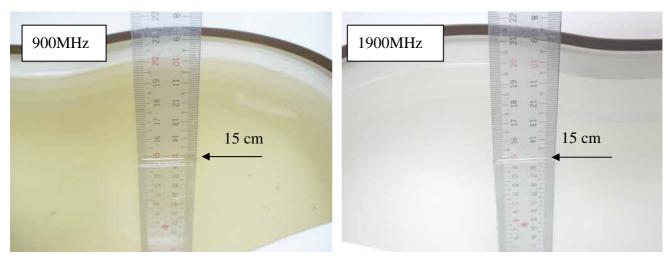


Fluid liquid depth 15cm for Left-head Side

Fig.2.1 Photograph of the Tissue Simulant Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side


Page: 3 of 26

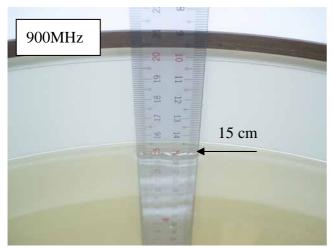

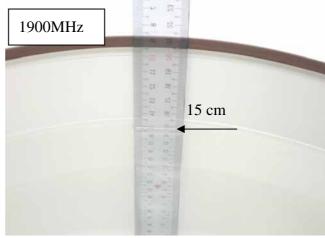

Fluid liquid depth 15cm for Flat (Body)

Fig.2-3 Photograph of the Tissue Simulant Fig.2-4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

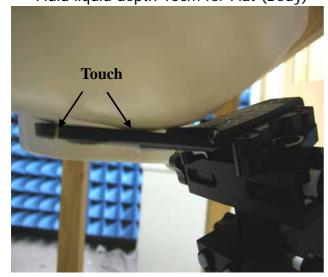

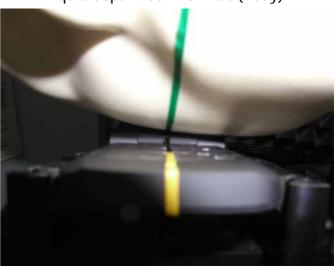


Fig.3 Right Head Section / Cheek-Touch Position

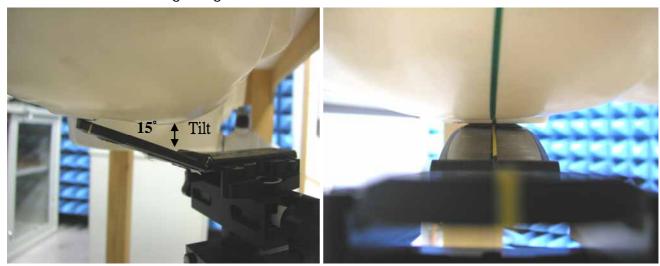


Fig.4 Right Head Section / Ear-Tilt Position(15°)

Report No. : ES/2006/20002 Page : 4 of 26

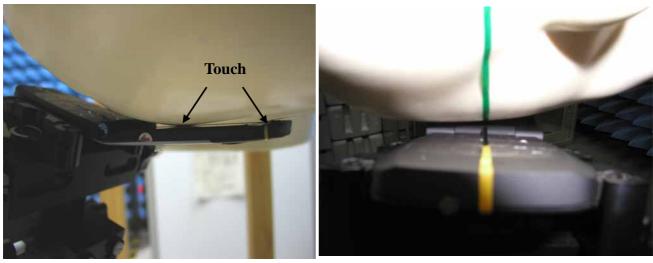


Fig.5 Left Head Section / Cheek-Touch Position

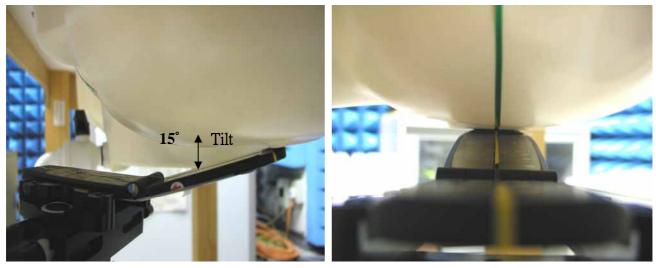


Fig.6 Left Head Section / Ear-Tilt Position(15°)

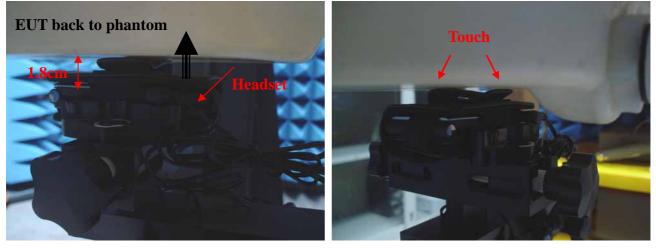


Fig. 7 Body position with belt clip and EUT back to phantom (testing in EDGE&GPRS Mode) , distance between flat phantom and mobile phone is 1.8 cm

Page: 5 of 26

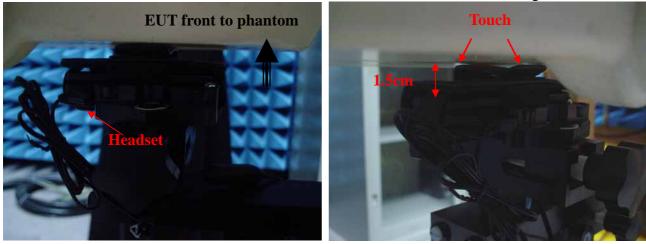


Fig.8 Body position with belt clip and EUT front to phantom (testing in EDGE&GPRS Mode) , distance between flat phantom and mobile phone is 1.5 cm

Report No. : ES/2006/20002 Page : 6 of 26

Photographs of the EUT



Fig.9 Front view of device



Fig.10 Back view of device with thin battery

Report No. : ES/2006/20002 Page : 7 of 26



Fig.11 Back view of device with thick battery



Fig.12 Open view of device

Report No. : ES/2006/20002 Page : 8 of 26



Fig.13 Side view of device with thin battery



Fig.14 Side view of device with thick battery

Page: 9 of 26

Photographs of the Battery



Fig.15 Front view of thin Battery (model: 160)



Fig.16 Front view of thick Battery (model: 161)

Page: 10 of 26



Fig.17 Black view of thin Battery (model: 160)



Fig.18 Black view of thick Battery (model: 161)

Report No. : ES/2006/20002 Page : 11 of 26

Photographs of the Accessories



Fig.19 Front view of belt clip



Fig.20 Black view of belt clip

Report No. : ES/2006/20002 Page : 12 of 26



Fig.21 side view of belt clip



Fig.22 Headset connect to EUT

Page: 13 of 26

Probe Calibration certificate

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client SGS (Auden)



Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Certificate No: ET3-1759 Aug05

Power sensor E4412A My41495277 3-May-05 (METAS, No. 251-00466) May-06 May-06 Reference 3 dB Attenuator SN: S5054 (3c) 11-Aug-05 (METAS, No. 251-00499) Aug-06 Reference 20 dB Attenuator SN: S5086 (20b) 3-May-05 (METAS, No. 251-00499) Aug-06 Reference 30 dB Attenuator SN: S5086 (20b) 3-May-05 (METAS, No. 251-00467) May-06 Reference 30 dB Attenuator SN: S5129 (30b) 11-Aug-05 (METAS, No. 251-00500) Aug-06 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) Jan-06 DAE4 SN: 654 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Nov-05 RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Dec-03) In house check: Dec-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) Name Function Signature Calibrated by:				
Calibration procedure for dosimetric E-field probes Calibration date: August 30, 2005 Condition of the calibrated item In Tolerance Chis calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards D #	Dbject	ET3DV6 - SN:1	759	
In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 3-May-05 (METAS, No. 251-00466) May-06 Power sensor E4412A MY41495277 3-May-05 (METAS, No. 251-00466) May-06 Power sensor E4412A MY41498087 3-May-05 (METAS, No. 251-00466) May-06 Reference 3 dB Attenuator SN: \$5054 (3c) 11-Aug-05 (METAS, No. 251-00467) Reference 20 dB Attenuator SN: \$5086 (20b) 3-May-05 (METAS, No. 251-00467) May-06 Reference 30 dB Attenuator SN: \$5129 (30b) 11-Aug-05 (METAS, No. 251-00500) Aug-06 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) Jan-06 Reference Probe ES3DV2 SN: 654 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Nov-05 Secondary Standards ID # Check Date (in house) Scheduled Check Reference The 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Dec-03) In house check: Dec-05 In house check: Nov 05 Name Function Signature Calibrated by:	Calibration procedure(s)	AT THE OWNER OF THE PROPERTY OF THE PROPERTY OF THE PARTY	edure for dosimetric E-field probes	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. It calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Trimary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Dever meter E4419B GB41293874 3-May-05 (METAS, No. 251-00466) May-06 Prower sensor E4412A MY41498087 3-May-05 (METAS, No. 251-00466) May-06 Reference 3 dB Attenuator SN: \$5054 (3c) 11-Aug-05 (METAS, No. 251-00499) Aug-06 Reference 20 dB Attenuator SN: \$5056 (20b) 3-May-05 (METAS, No. 251-00467) May-06 Reference 30 dB Attenuator SN: \$5129 (30b) 11-Aug-05 (METAS, No. 251-00467) May-06 Reference 30 dB Attenuator SN: \$5129 (30b) 11-Aug-05 (METAS, No. 251-00467) May-06 Reference 20 dB Attenuator SN: \$5129 (30b) 11-Aug-05 (METAS, No. 251-00500) Aug-06 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. E93-3013_Jan05) Jan-06 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. DAE4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 3013 Robert Check Date (in house) Scheduled Check Recondary Standards ID # Check Date (in house check Dec-03) In house check: Dec-05 In house check: Nov 05 Name Function Signature Name Name Function Signature	Calibration date:	August 30, 2005		
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards D #	Condition of the calibrated item	In Tolerance		
Power meter E4419B GB41293874 3-May-05 (METAS, No. 251-00466) May-06 May-0				d humidity < 70%.
Power sensor E4412A My41495277 3-May-05 (METAS, No. 251-00466) May-06 May-06 Reference 3 dB Attenuator Reference 20 dB Attenuator SN: S5054 (3c) 11-Aug-05 (METAS, No. 251-00499) Aug-06 Reference 20 dB Attenuator SN: S5086 (20b) 3-May-05 (METAS, No. 251-00467) May-06 Reference 30 dB Attenuator SN: S5129 (30b) 11-Aug-05 (METAS, No. 251-00467) May-06 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) Jan-06 DAE4 SN: 654 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. DAE4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 654 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 654 10-D4E4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 654 10-D4E4-654_Nov04) Nov-05 Reference Probe ES3DV2 SN: 654 10-D4E4-654_Nov04) Nov-05 Nov-05 Network Analyzer HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Dec-03) In house check: Dec-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov 05 Name Function Signature Nico Vetterlii Laboratory Technician				0.1.1.1.0.15
Name	Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	
SN: S5054 (3c) 11-Aug-05 (METAS, No. 251-00499) Aug-06	Primary Standards Power meter E4419B	ID # GB41293874	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466)	May-06
Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 Reference 20 dB Attenuator Referenc	Primary Standards Power meter E4419B Power sensor E4412A	ID# GB41293874 MY41495277	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06
Reference 30 dB Attenuator Reference Probe ES3DV2 Reference 30 dB Attenuator Reference 30 dB Attenua	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ID # GB41293874 MY41495277 MY41498087	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06 May-06
Reference Probe ES3DV2 SN: 3013 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) Jan-06 Nov-05 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C Network Analyzer HP 8753E US37390585 Name Function Signature Calibrated by: SN: 3013 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) Jan-06 Nov-05	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00499)	May-06 May-06 May-06 Aug-06
Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Dec-03) In house check: Dec-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov 05 Name Function Signature Calibrated by: Nico Vetterli Laboratory Technician	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No. 251-00497) 3-May-05 (METAS, No. 251-00467)	May-06 May-06 May-06 Aug-06 May-06
RF generator HP 8648C Network Analyzer HP 8753E US3642U01700 US37390585 US37390585 Name Function Signature Calibrated by: US3642U01700 4-Aug-99 (SPEAG, in house check Dec-03) In house check: Dec-05 In house check: Nov 05 Signature Laboratory Technician	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500)	May-06 May-06 May-06 Aug-06 May-06 Aug-06
Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov 05 Name Function Signature Calibrated by: Laboratory Technician	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Jan-06
Name Function Signature Calibrated by: Laboratory Technician	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Jan-06 Nov-05
Calibrated by: Laboratory Technician Odder	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No. 251-00497) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Jan-06 Nov-05 Scheduled Check In house check: Dec-05
Nichell	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No. 251-00497) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03)	May-06 May-06 May-06 Aug-06 May-06 Aug-06 Jan-06 Nov-05 Scheduled Check In house check: Dec-05
Approved by: Katja Pokovic Technical Manager	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04)	May-06 May-06 May-06 Aug-06 Aug-06 Jan-06 Nov-05 Scheduled Check In house check: Dec-05 In house check: Nov 05
	Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 7-Jan-05 (SPEAG, No. ES3-3013_Jan05) 29-Nov-04 (SPEAG, No. DAE4-654_Nov04) Check Date (in house) 4-Aug-99 (SPEAG, in house check Dec-03) 18-Oct-01 (SPEAG, in house check Nov-04)	May-06 May-06 May-06 Aug-06 Aug-06 Jan-06 Nov-05 Scheduled Check In house check: Dec-05 In house check: Nov 05

Page: 14 of 26

Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates



Schweizerischer Kalibrierdienst

Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConF sensitivity in TSL / NORMx,y,z

ConF sensitivity in TSL / NORMx,y
DCP diode compression point
Polarization φ rotation around probe axis

Polarization ϑ ϑ rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Page: 15 of 26

ET3DV6 SN:1759

August 30, 2005

Probe ET3DV6

SN:1759

Manufactured:

Last calibrated:

Repaired: Recalibrated:

November 12, 2002

March 23, 2005

July 28, 2005

August 30, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Page: 16 of 26

ET3DV6 SN:1759 August 30, 2005

DASY - Parameters of Probe: ET3DV6 SN:1759

Sensitivity	Sensitivity in Free Space ^A			Diode C	ompression ^B
Norn	nX	1.97 ± 10.1%	μ V/(V/m) ²	DCP X	93 mV
Norn	nΥ	1.90 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
Norn	nZ	1.93 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	93 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	8.3	4.7
SAR _{be} [%]	With Correction Algorithm	0.0	0.2

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	13.4	9.2
SAR _{be} [%]	With Correction Algorithm	0.8	0.2

Sensor Offset

Probe Tip to Sensor Center 2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Page 8).

^B Numerical linearization parameter: uncertainty not required.


Page: 17 of 26

ET3DV6 SN:1759

August 30, 2005

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

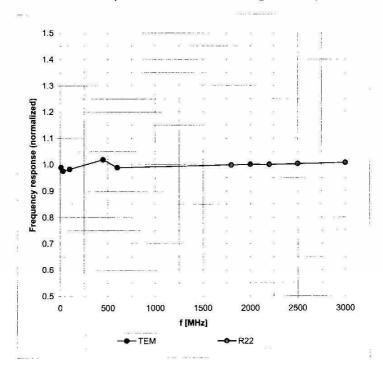


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Report No. : ES/2006/20002 Page : 18 of 26


ET3DV6 SN:1759

August 30, 2005

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

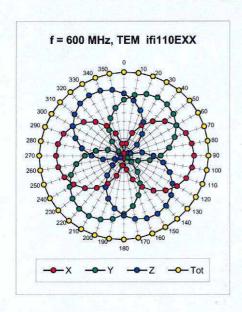



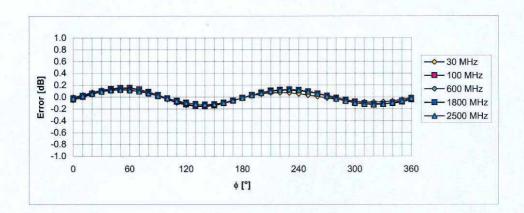

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Page: 19 of 26


ET3DV6 SN:1759

August 30, 2005

Dynamic Range f(SAR_{head})

(Waveguide R22, f = 1800 MHz)

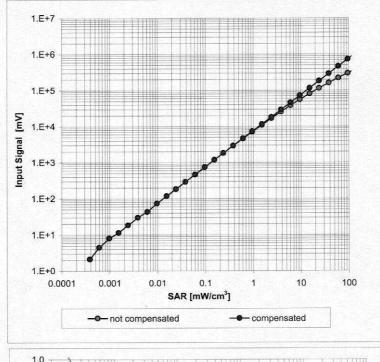

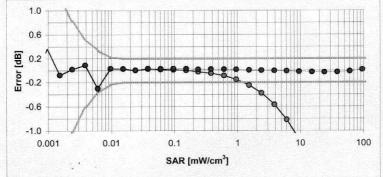


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Report No. : ES/2006/20002 Page : 20 of 26

ET3DV6 SN:1759

August 30, 2005

Conversion Factor Assessment

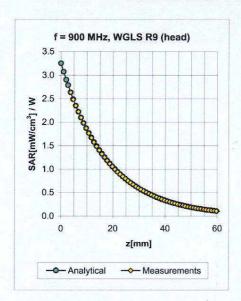



f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.48	2.00	6.15 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.58	2.42	5.11 ± 11.0% (k=2)
2000	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.58	2.56	4.72 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.69	2.15	4.39 ± 11.8% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.46	2.16	5.93 ± 11.0% (k=2)
1750	± 50 / ± 100 ± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.46	2.87	4.40 ± 11.0% (k=2)
1900	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.53	2.98	4.33 ± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.59	2.54	4.20 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.70	1.95	4.08 ± 11.8% (k=2)

 $^{^{\}mathrm{C}}$ The validity of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Report No. : ES/2006/20002 Page : 21 of 26

Uncertainty Analysis

DASY4 Uncertainty Budget According to IEEE P1528 [1]

	Uncertainty	Prob.	Div.	(c_i)	(c_i)	Std. Unc.	Std. Unc.	(v_i)
Error Description	value	Dist.		1g	10g	(1g)	(10g)	v_{eff}
Measurement System								
Probe Calibration	±4.8 %	N	1	1	1	±4.8 %	±4.8 %	∞
Axial Isotropy	±4.7 %	R	$\sqrt{3}$	0.7	0.7	$\pm 1.9 \%$	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	R	$\sqrt{3}$	0.7	0.7	$\pm 3.9 \%$	$\pm 3.9 \%$	∞
Boundary Effects	±1.0 %	R	$\sqrt{3}$	1	1	±0.6 %	±0.6 %	∞
Linearity	$\pm 4.7 \%$	R	$\sqrt{3}$	1	1	$\pm 2.7 \%$	±2.7 %	∞
System Detection Limits	$\pm 1.0 \%$	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	$\pm 0.6 \%$	∞
Readout Electronics	±1.0 %	N	1	1	1	±1.0%	±1.0 %	∞
Response Time	±0.8 %	R	$\sqrt{3}$	1	1	$\pm 0.5 \%$	$\pm 0.5\%$	∞
Integration Time	±2.6 %	R	$\sqrt{3}$	1	1	$\pm 1.5 \%$	$\pm 1.5 \%$	∞
RF Ambient Conditions	±3.0 %	R	$\sqrt{3}$	1	1	$\pm 1.7 \%$	$\pm 1.7 \%$	∞
Probe Positioner	$\pm 0.4\%$	R	$\sqrt{3}$	1	1	$\pm 0.2 \%$	$\pm 0.2 \%$	∞
Probe Positioning	$\pm 2.9 \%$	R	$\sqrt{3}$	1	1	$\pm 1.7 \%$	$\pm 1.7 \%$	∞
Max. SAR Eval.	$\pm 1.0 \%$	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	$\pm 0.6 \%$	∞
Test Sample Related								
Device Positioning	±2.9 %	N	1	1	1	$\pm 2.9 \%$	±2.9 %	875
Device Holder	±3.6 %	N	1	1	1	$\pm 3.6 \%$	±3.6 %	5
Power Drift	±5.0 %	R	$\sqrt{3}$	1	1	$\pm 2.9 \%$	±2.9 %	∞
Phantom and Setup								
Phantom Uncertainty	±4.0 %	R	$\sqrt{3}$	1	1	$\pm 2.3 \%$	$\pm 2.3 \%$	∞
Liquid Conductivity (target)	±5.0 %	R	$\sqrt{3}$	0.64	0.43	$\pm 1.8 \%$	$\pm 1.2 \%$	∞
Liquid Conductivity (meas.)	±2.5 %	N	1	0.64	0.43	$\pm 1.6 \%$	±1.1 %	∞
Liquid Permittivity (target)	±5.0 %	R	$\sqrt{3}$	0.6	0.49	$\pm 1.7 \%$	$\pm 1.4 \%$	∞
Liquid Permittivity (meas.)	$\pm 2.5 \%$	N	1	0.6	0.49	$\pm 1.5 \%$	$\pm 1.2 \%$	∞
Combined Std. Uncertainty						$\pm 10.3 \%$	±10.0 %	331
Expanded STD Uncertain	tv				16	$\pm 20.6\%$	$\pm 20.1\%$	

Page: 22 of 26

Phantom description

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

Item .	SAM Twin Phantom V4.0		
Type No	QD 000 P40 CA		100
Series No	TP-1150 and higher	٥	_
Manufacturer / Origin -	Untersee Composites		
	Hauntstr. 69	× 5 × .	i .
3.	CH-8559 Fruthwilen	*	
	Switzerland		

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

		Details	Units tested
Test Shape	Requirement Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm ln specific areas	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05.	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards	Liquid type HSL 1800	Pre-series, First article

Standards

[1] CENELEC!	EN 50361
--------------	----------

[2] IEEE P1528-200x draft 6.5

[3] *IEC PT 62209 draft 0.9

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date

28.02.2002

Signature / Stamp

Schmid & Partner Engineering AG

Zoughausstracce 43, CH-8004 Zurich Tel. +41 1 245 97 00, Fax +41 1 245 97 74

F. Rombult

Page: 23 of 26

System Validation from Original equipment supplier SPEAG Schmid & Partner of GSM 900MHz & 1900MHz (HSL& Muscle)

DASY4 Validation Report for Head TSL

Date/Time: 06.02.2006 15:37:06

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:178

Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 900 MHz; $\sigma = 0.96 \text{ mho/m}$; $\varepsilon_r = 42.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

Probe: ET3DV6 - SN1507 (HF); ConvF(5.8, 5.8, 5.8); Calibrated: 28.10.2005

- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA
- Measurement SW: DASY4, V4.6 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 160

Pin = 250 mW; d = 10 mm/Area Scan (71x81x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 2.98 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.5 V/m; Power Drift = -0.123 dB

Peak SAR (extrapolated) = 4.15 W/kg

SAR(1 g) = 2.75 mW/g; SAR(10 g) = 1.77 mW/g

Maximum value of SAR (measured) = 2.98 mW/g

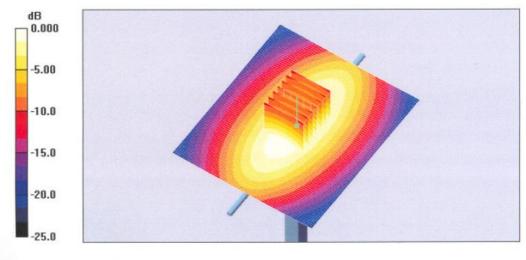

0 dB = 2.98 mW/g

Page: 24 of 26

DASY4 Validation Report for Body TSL

Date/Time: 07.02.2006 16:55:51

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:178

Communication System: CW900; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: MSL U10;

Medium parameters used: f = 900 MHz; $\sigma = 1$ mho/m; $\varepsilon_r = 56.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

Probe: ET3DV6 - SN1507 (HF); ConvF(5.76, 5.76, 5.76); Calibrated: 28.10.2005

• Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 15.12.2005

• Phantom: Flat Phantom 4.9L; Type: QD000P49AA

Measurement SW: DASY4, V4.6 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 160

Pin = 250 mW; d = 10 mm/Area Scan (71x81x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 2.81 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.0 V/m; Power Drift = -0.020 dB

Peak SAR (extrapolated) = 3.70 W/kg

SAR(1 g) = 2.57 mW/g; SAR(10 g) = 1.69 mW/g

Maximum value of SAR (measured) = 2.78 mW/g

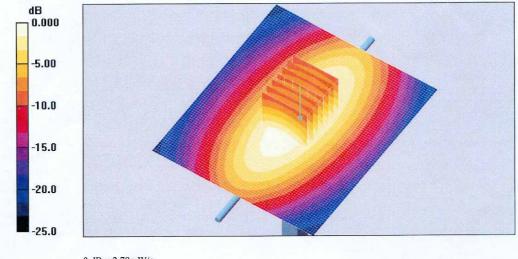

0~dB=2.78mW/g

Certificate No: D900V2-178_Feb06

Page: 25 of 26

DASY4 Validation Report for Head TSL

Date/Time: 13.06.2005 15:36:41

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d060

Communication System: CW-1900; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL 1900 MHz;

Medium parameters used: f = 1900 MHz; $\sigma = 1.45 \text{ mho/m}$; $\varepsilon_r = 39.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

Probe: ET3DV6 - SN1507; ConvF(4.96, 4.96, 4.96); Calibrated: 26.10.2004

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 07.01.2005

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA

Measurement SW: DASY4, V4.6 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 149

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 11.2 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 88.0 V/m; Power Drift = 0.081 dB

Peak SAR (extrapolated) = 17.2 W/kg

SAR(1 g) = 9.83 mW/g; SAR(10 g) = 5.13 mW/g

Maximum value of SAR (measured) = 11.2 mW/g

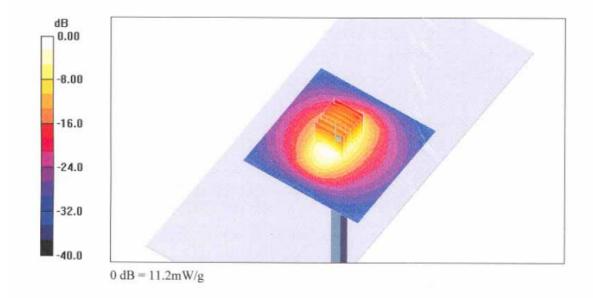

Report No. : ES/2006/20002 Page : 26 of 26

DASY4 Validation Report for Body TSL

Date/Time: 14.06.2005 15:16:42

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d060

Communication System: CW-1900; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL 1900 MHz;

Medium parameters used: f = 1900 MHz; $\sigma = 1.57$ mho/m; $\varepsilon_r = 52.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

Probe: ET3DV6 - SN1507; ConvF(4.43, 4.43, 4.43); Calibrated: 26.10.2004

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 07.01.2005

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA

Measurement SW: DASY4, V4.6 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 149

Pin = 250 mW; d = 10 mm 2/Area Scan (81x81x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 11.6 mW/g

Pin = 250 mW; d = 10 mm 2/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 86.7 V/m; Power Drift = 0.100 dB

Peak SAR (extrapolated) = 17.4 W/kg

SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.37 mW/g

Maximum value of SAR (measured) = 11.6 mW/g

