



### 3. Internal Photograph of EUT

Brand Name: Mio, Mitac,Stryker / Model Name: N450



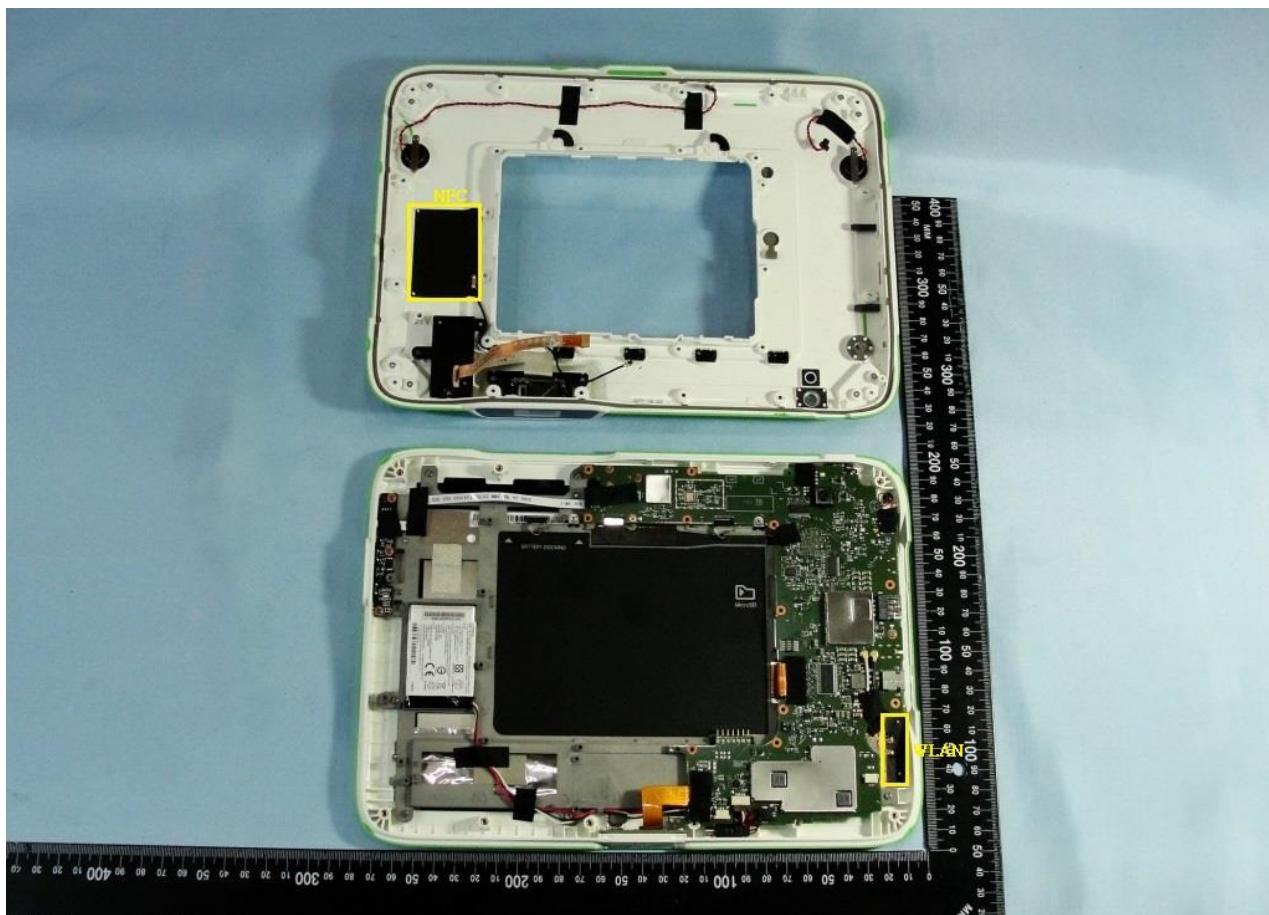


Brand Name: Mio, Mitac,Stryker / Model Name: N450

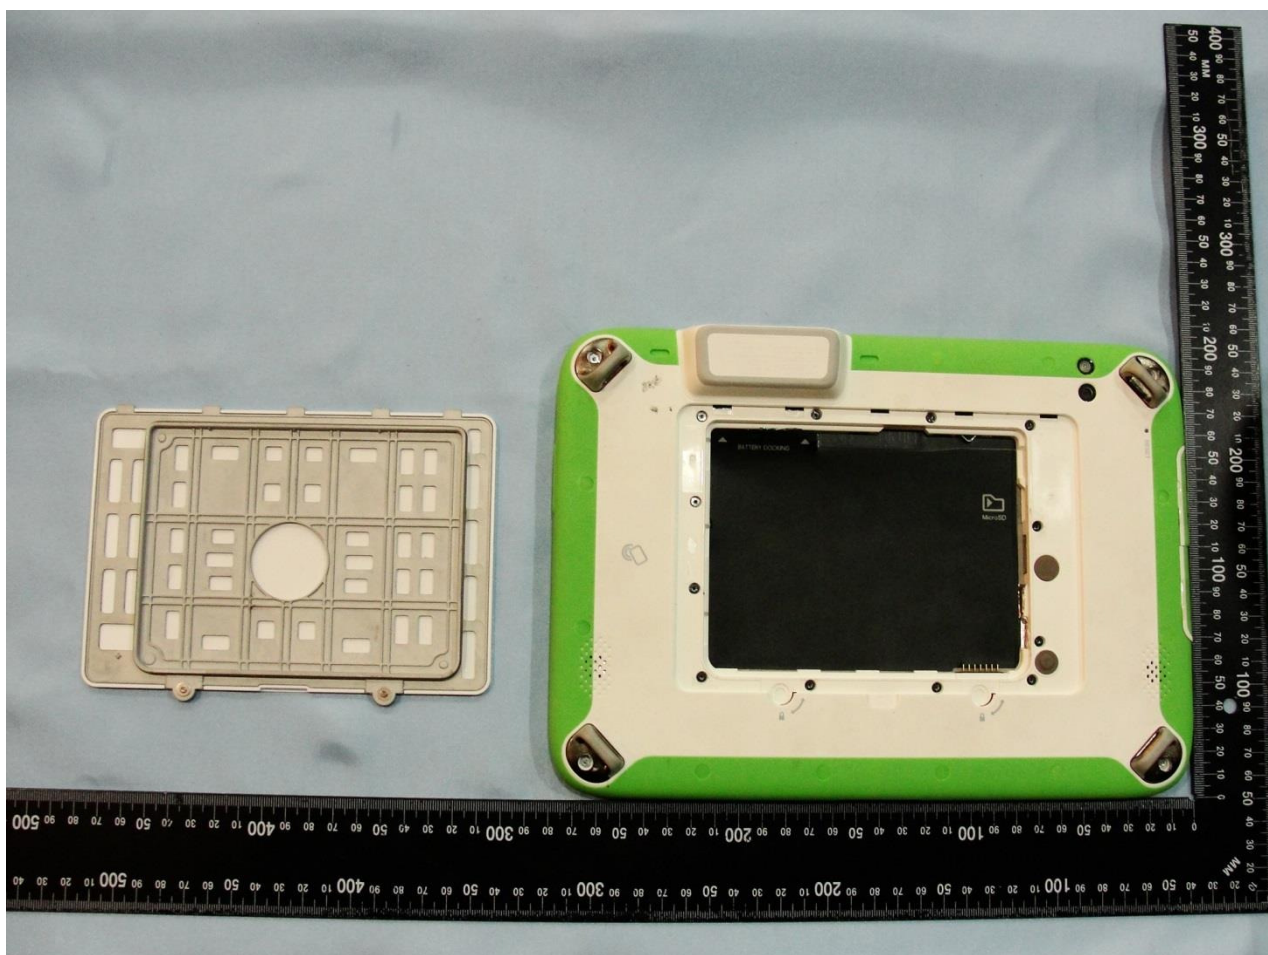




Brand Name: Mio, Mitac,Stryker / Model Name: N450

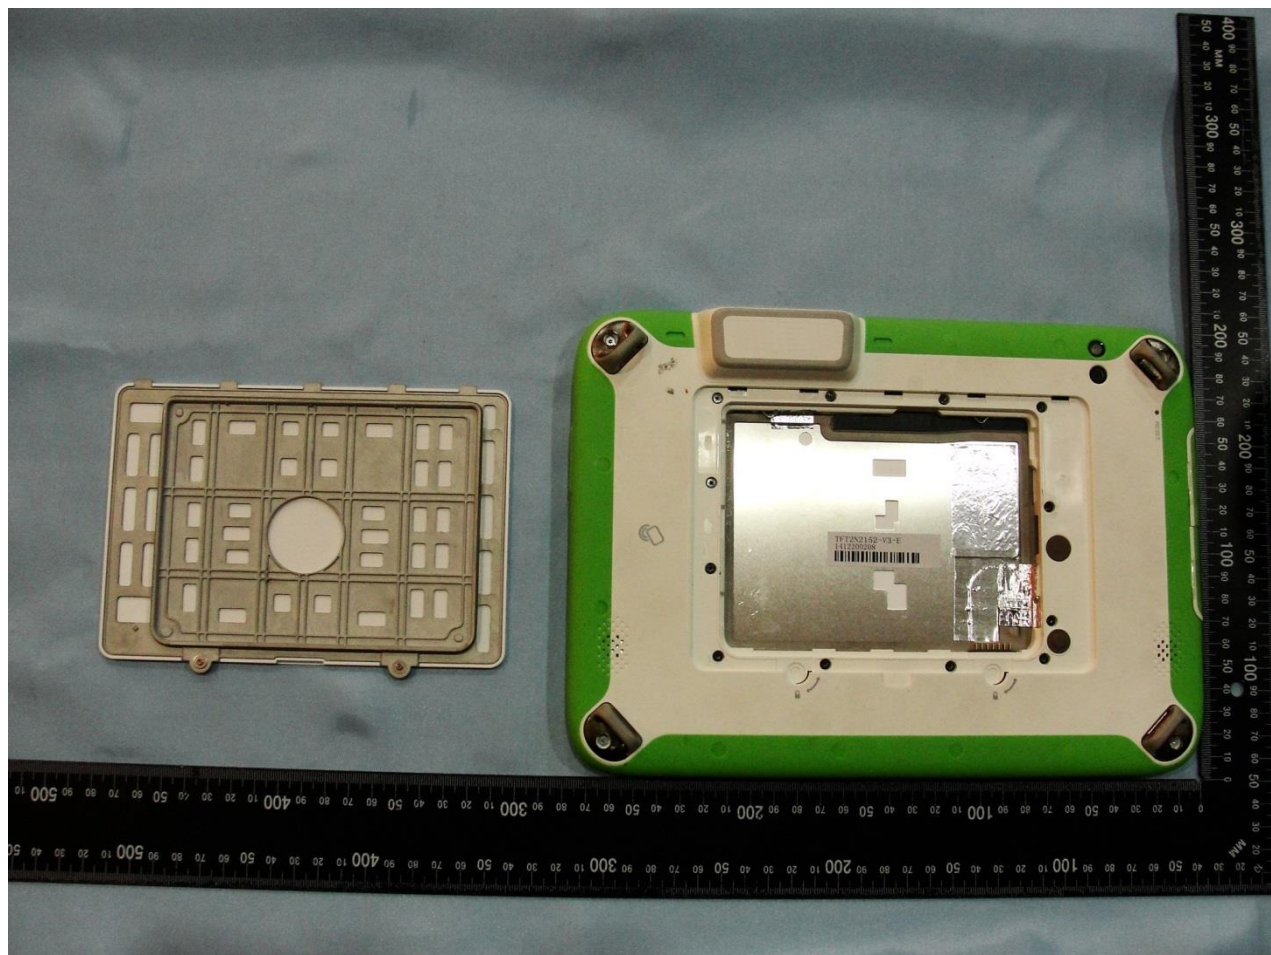




**Brand Name: Mio, Mitac,Stryker / Model Name: N450**

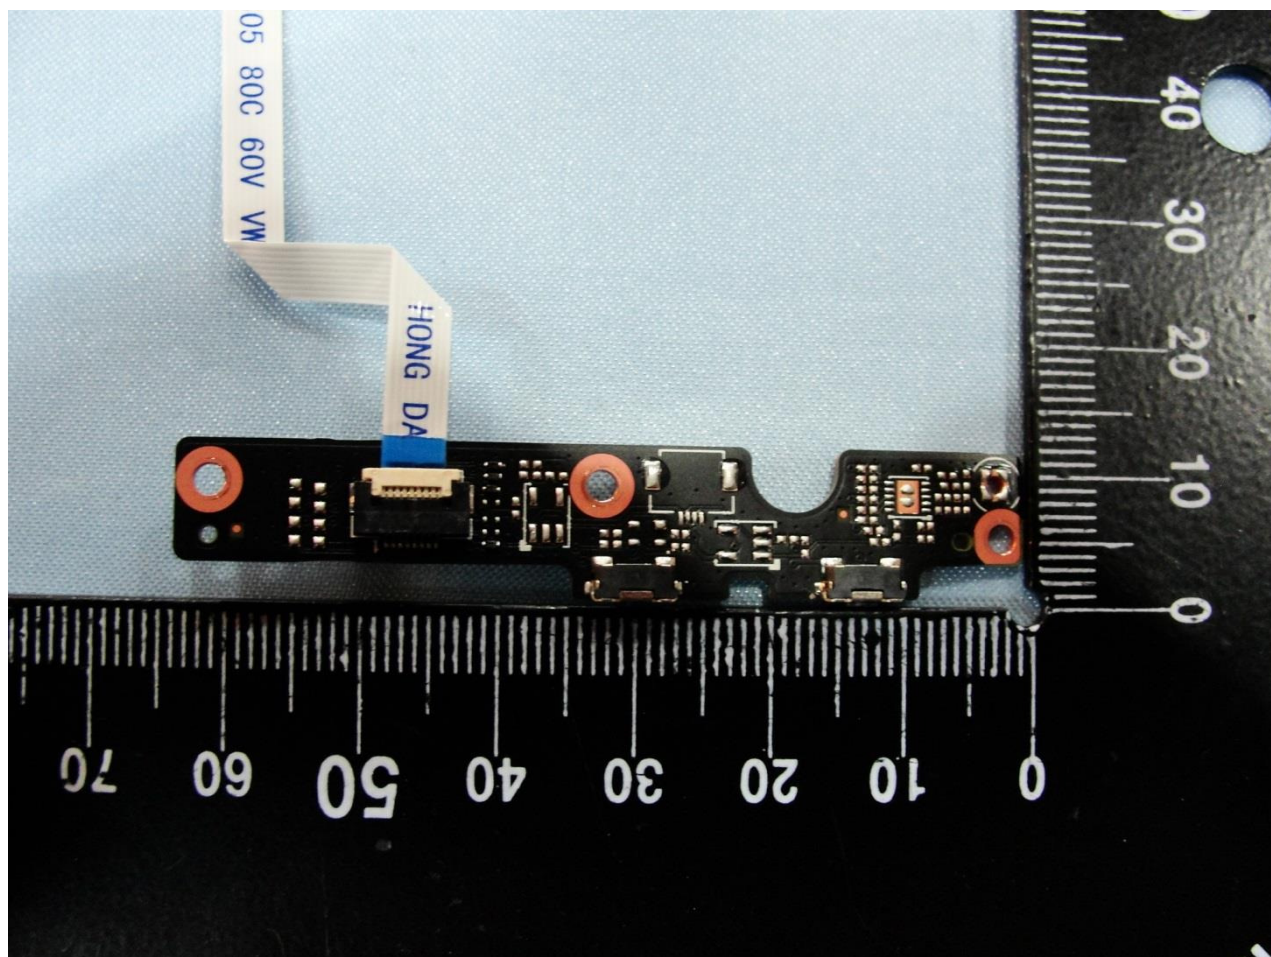




Brand Name: Mio, Mitac,Stryker / Model Name: N450

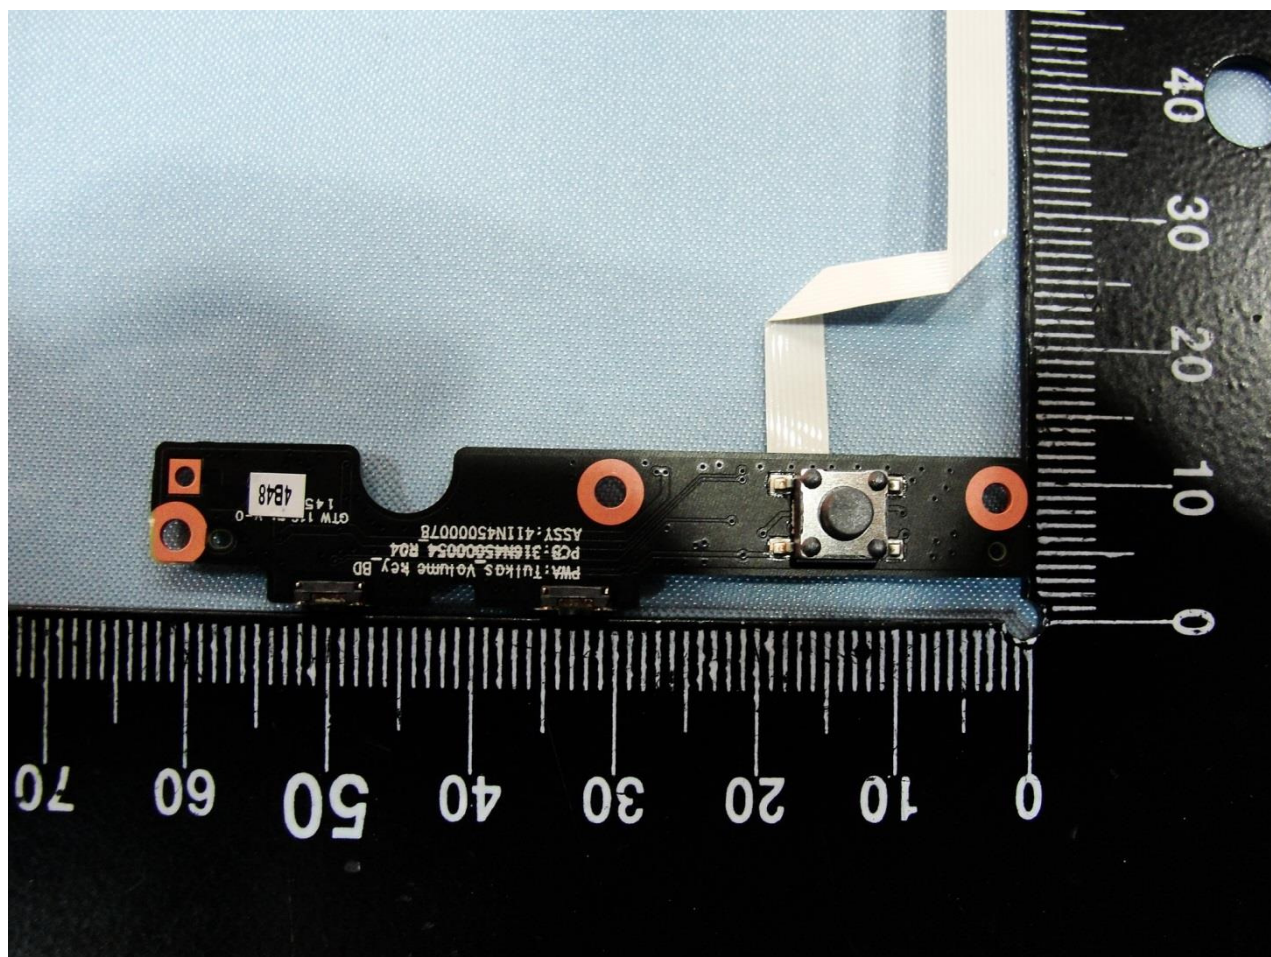






**Brand Name: Mio, Mitac, Stryker / Model Name: N450**

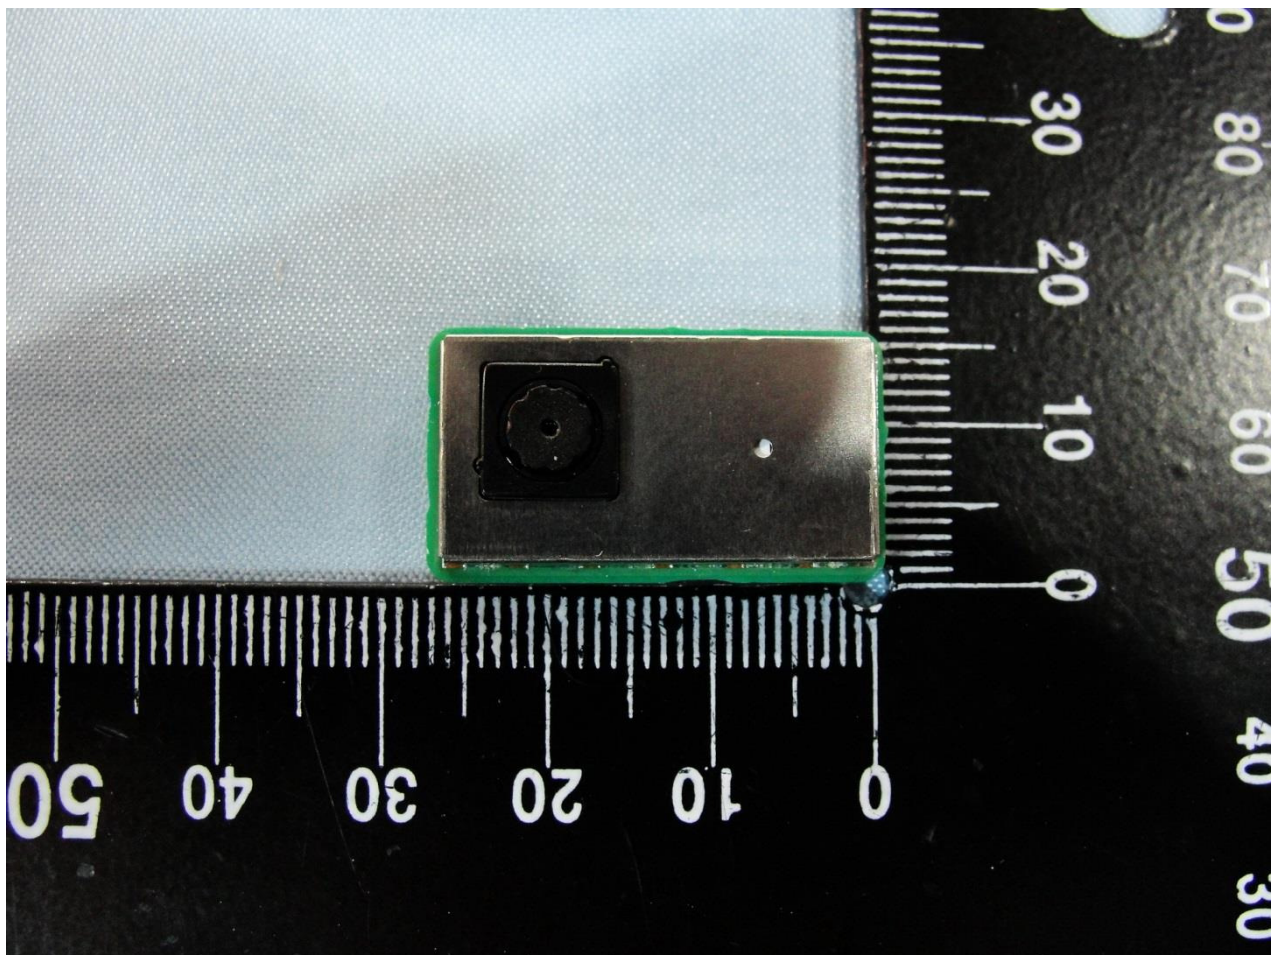


Brand Name: Mio, Mitac, Stryker / Model Name: N450

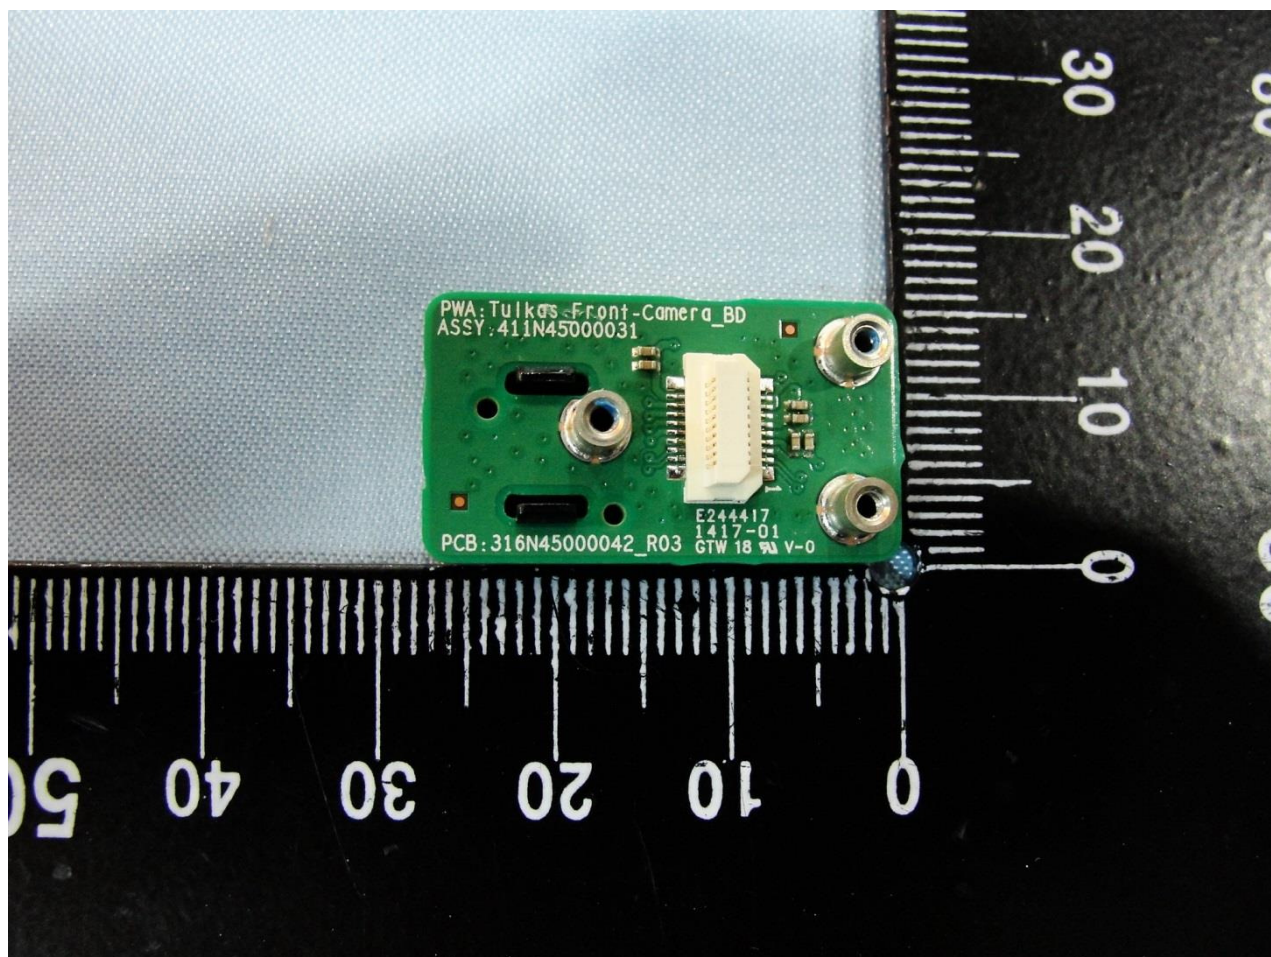






**Brand Name: Mio, Mitac, Stryker / Model Name: N450**

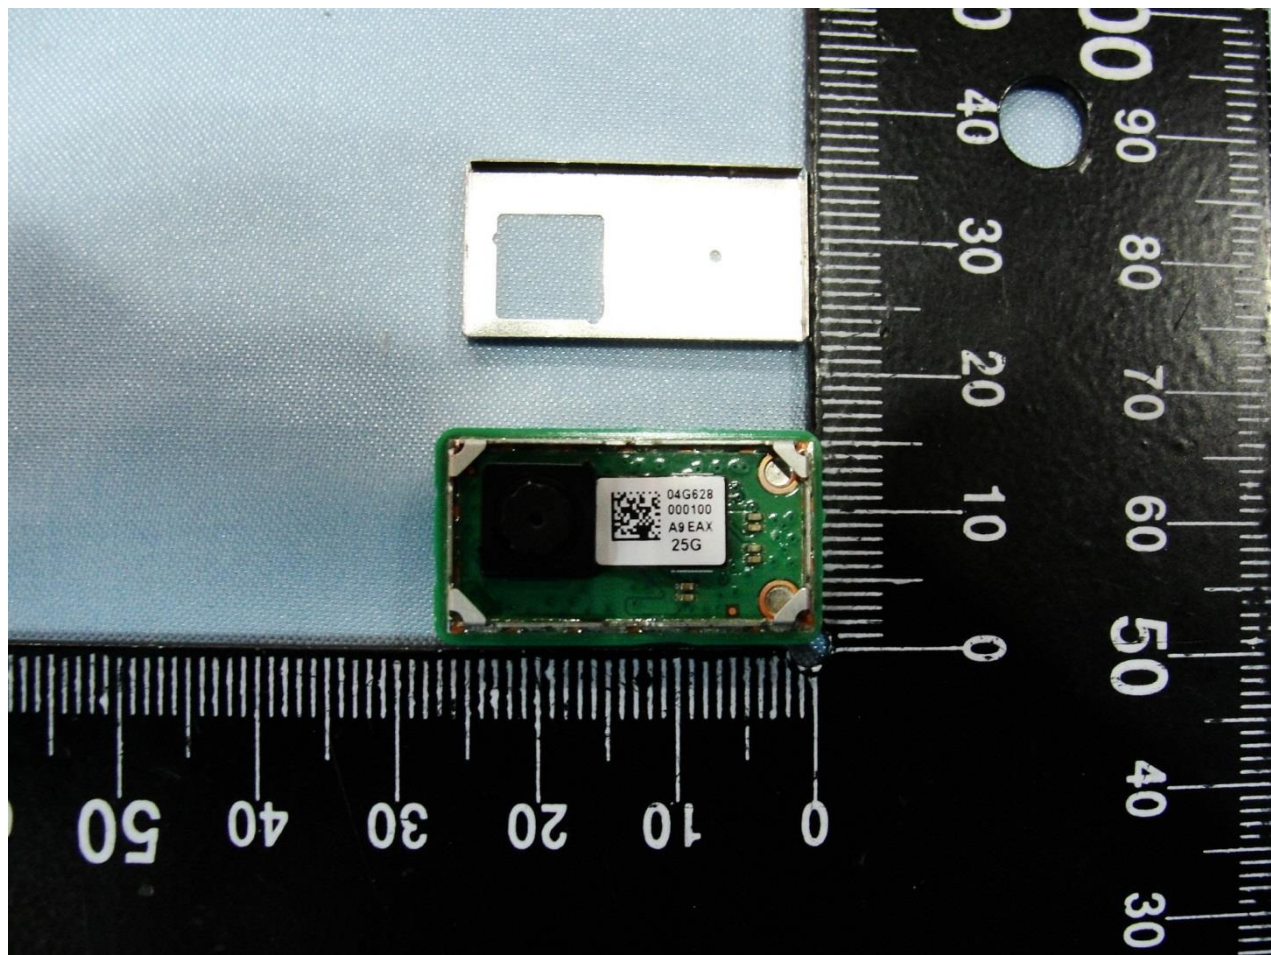




Brand Name: Mio, Mitac, Stryker / Model Name: N450

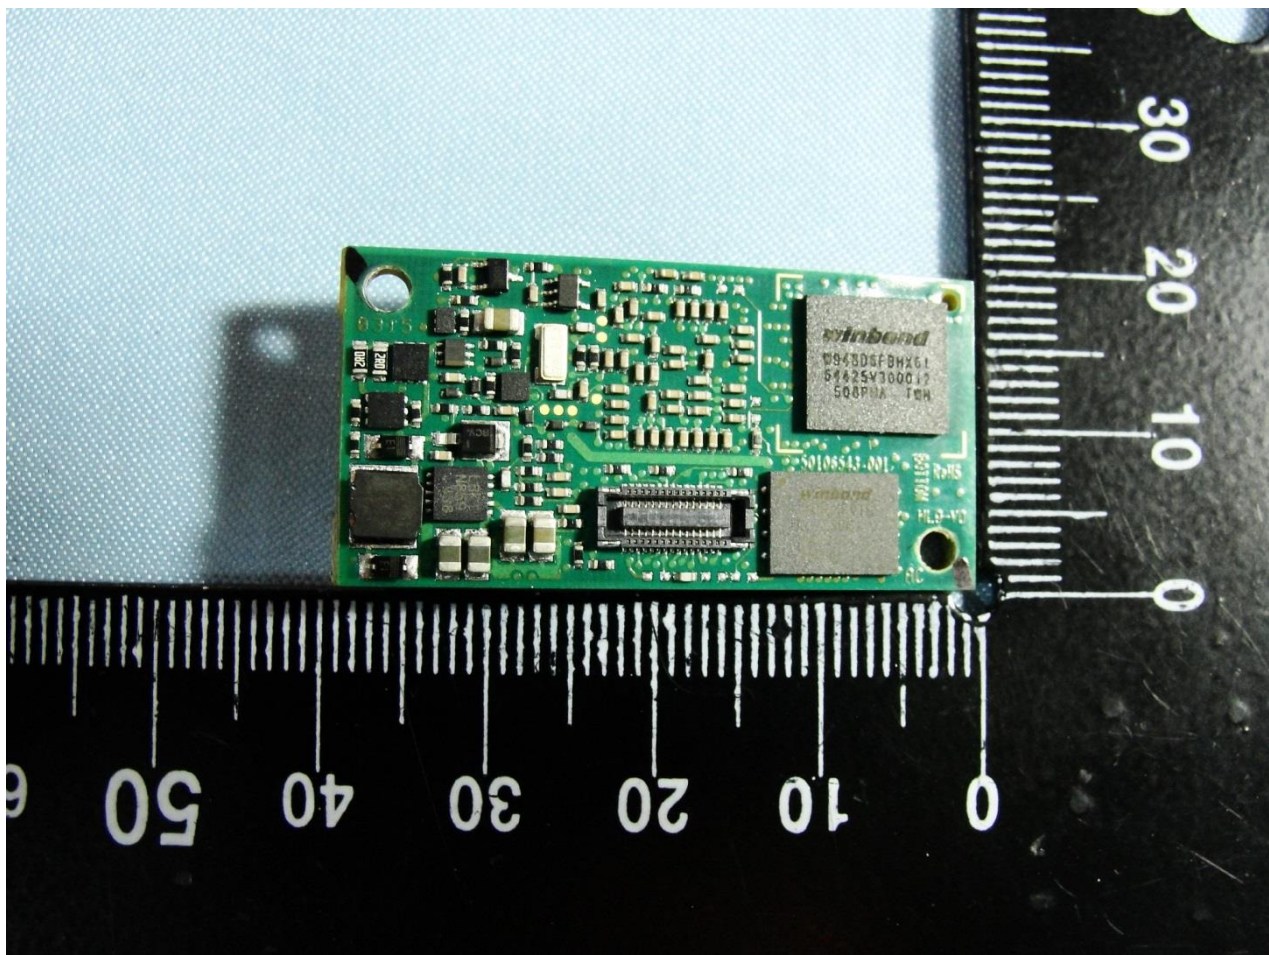


Brand Name: Mio, Mitac, Stryker / Model Name: N450

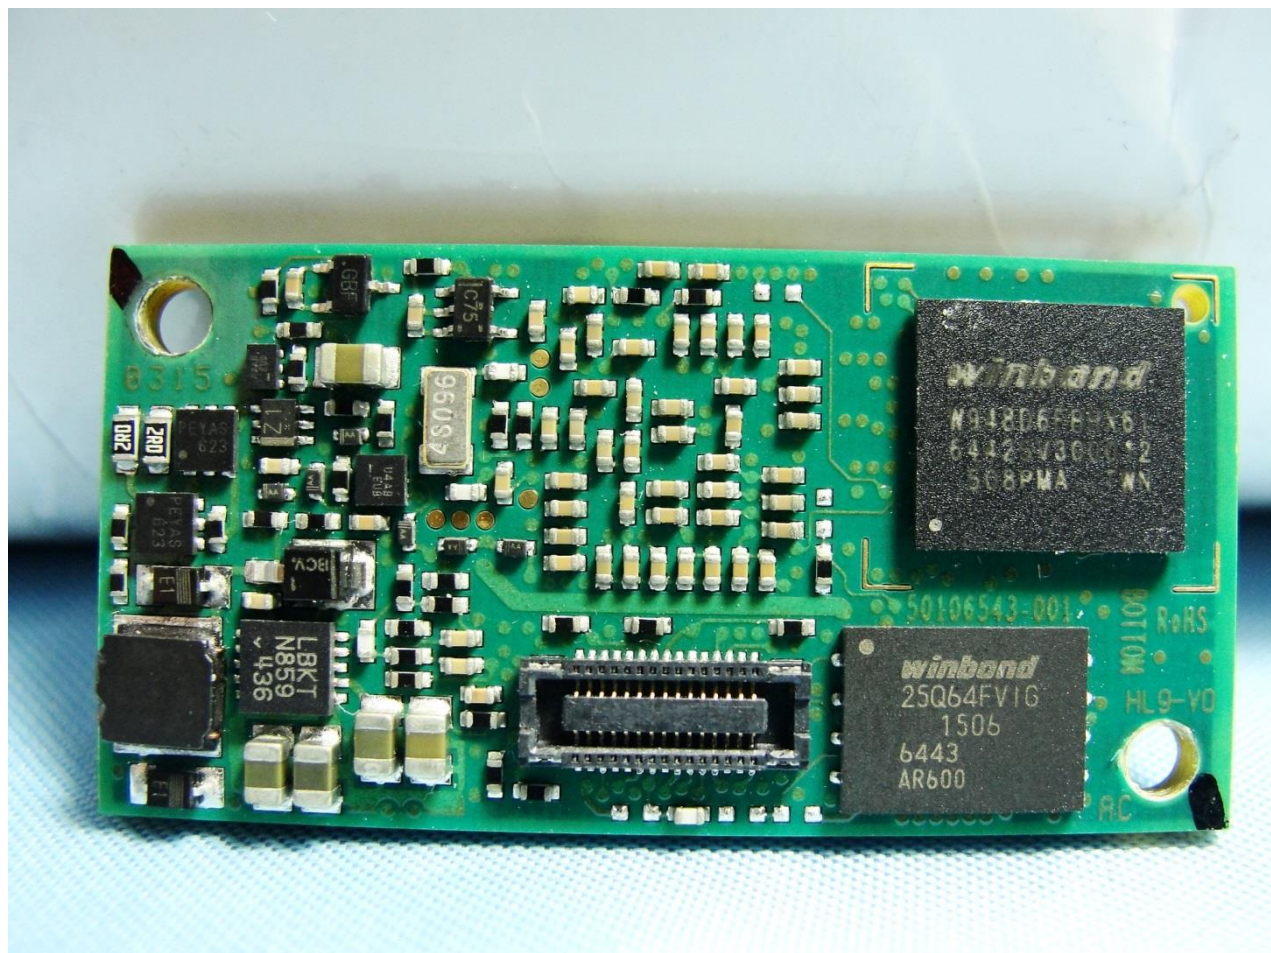




Brand Name: Mio, Mitac,Stryker / Model Name: N450

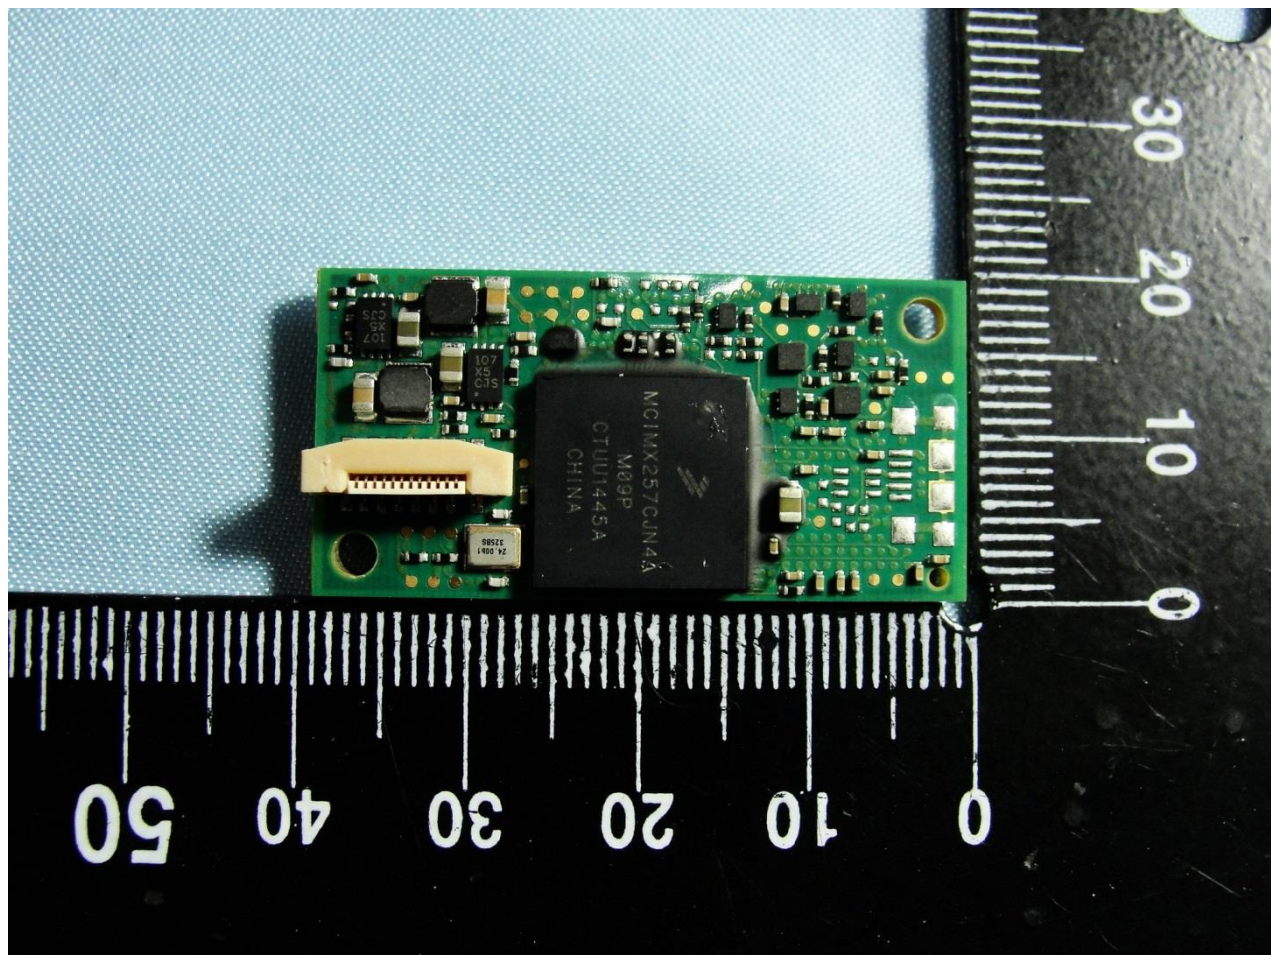




Brand Name: Mio, Mitac,Stryker / Model Name: N450

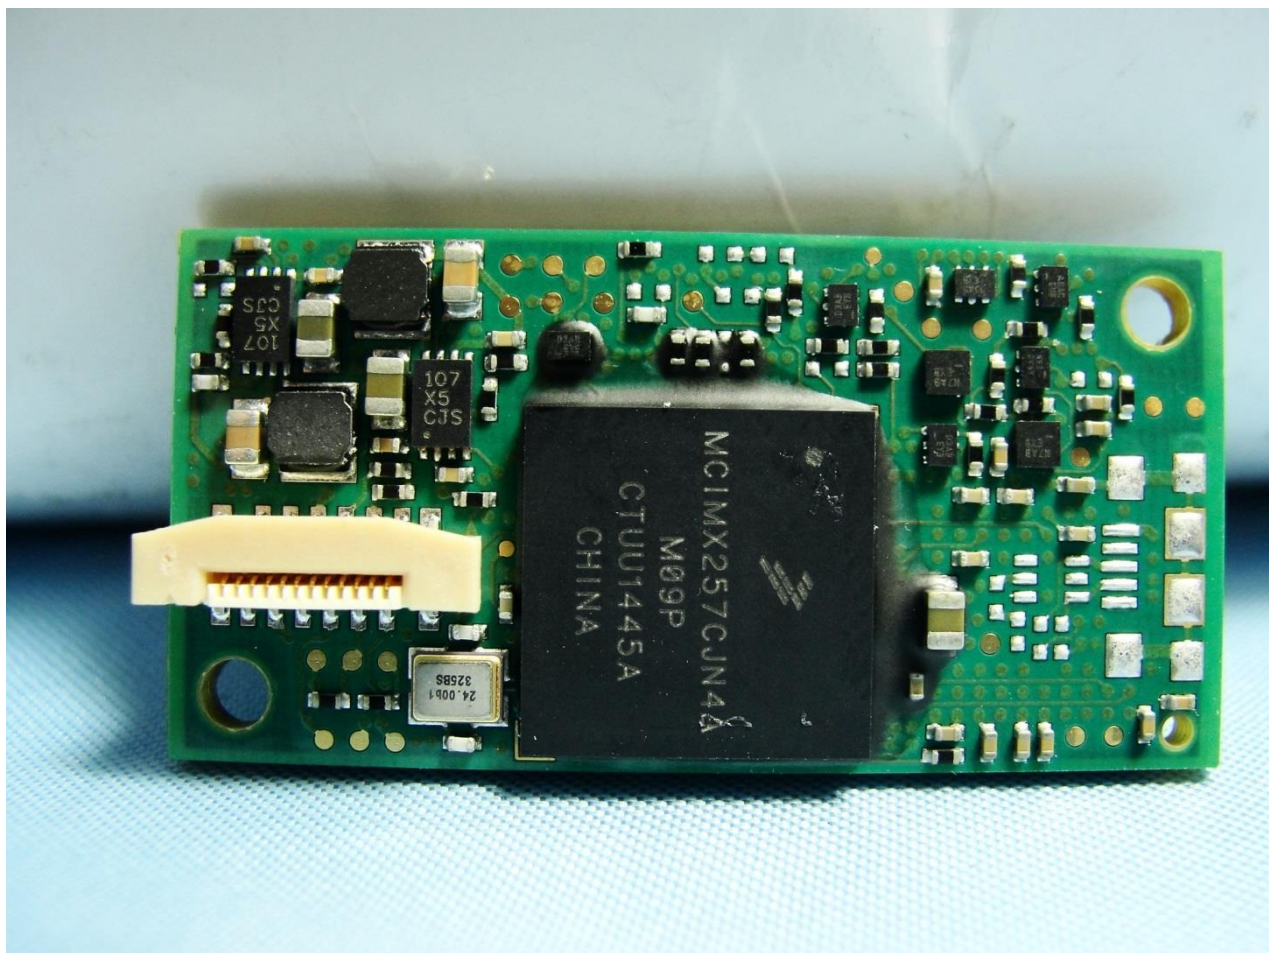





**Brand Name: Mio, Mitac,Stryker / Model Name: N450**

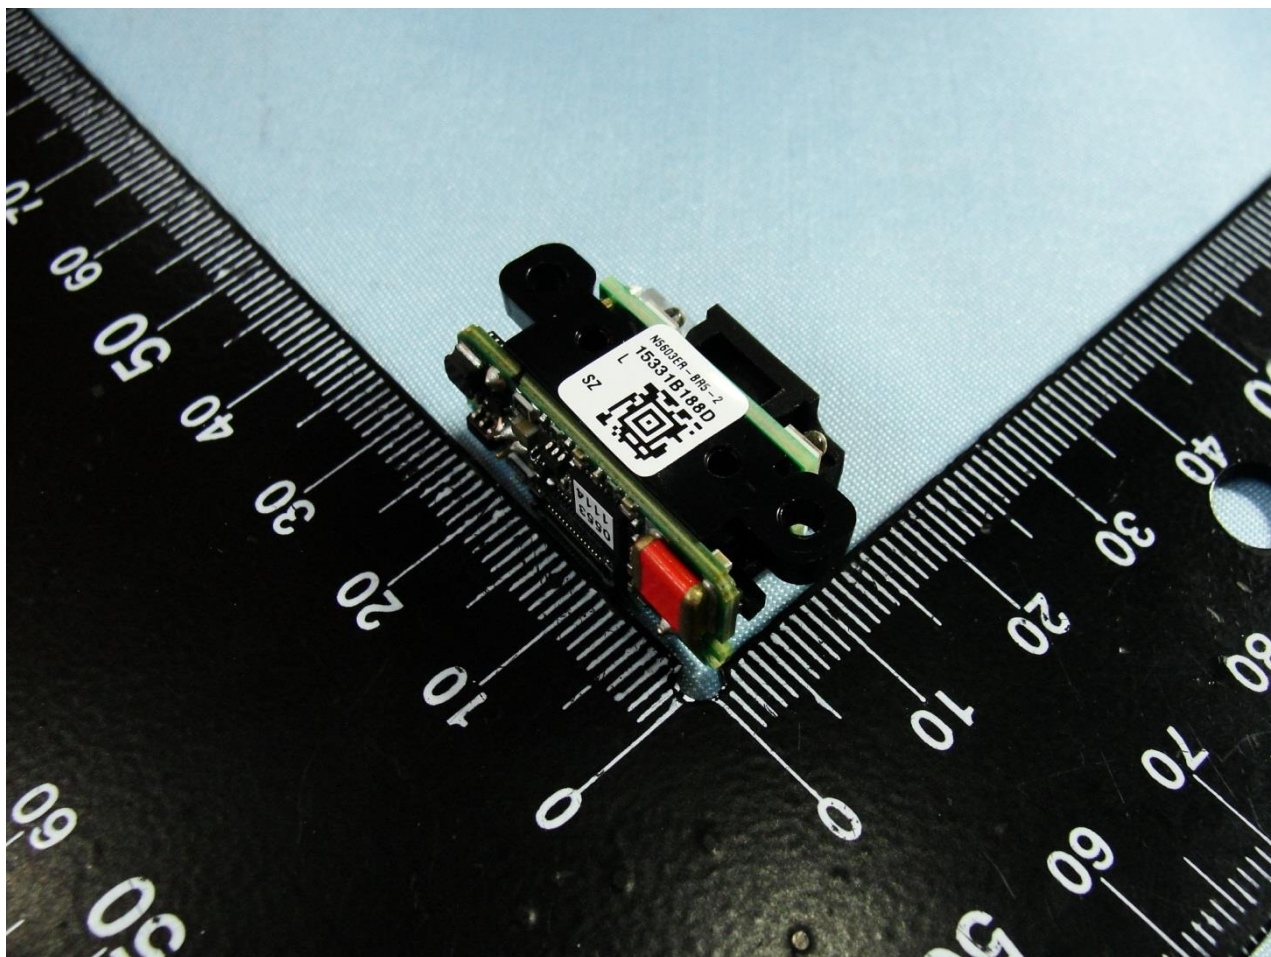



**Brand Name: Mio, Mitac, Stryker / Model Name: N450**

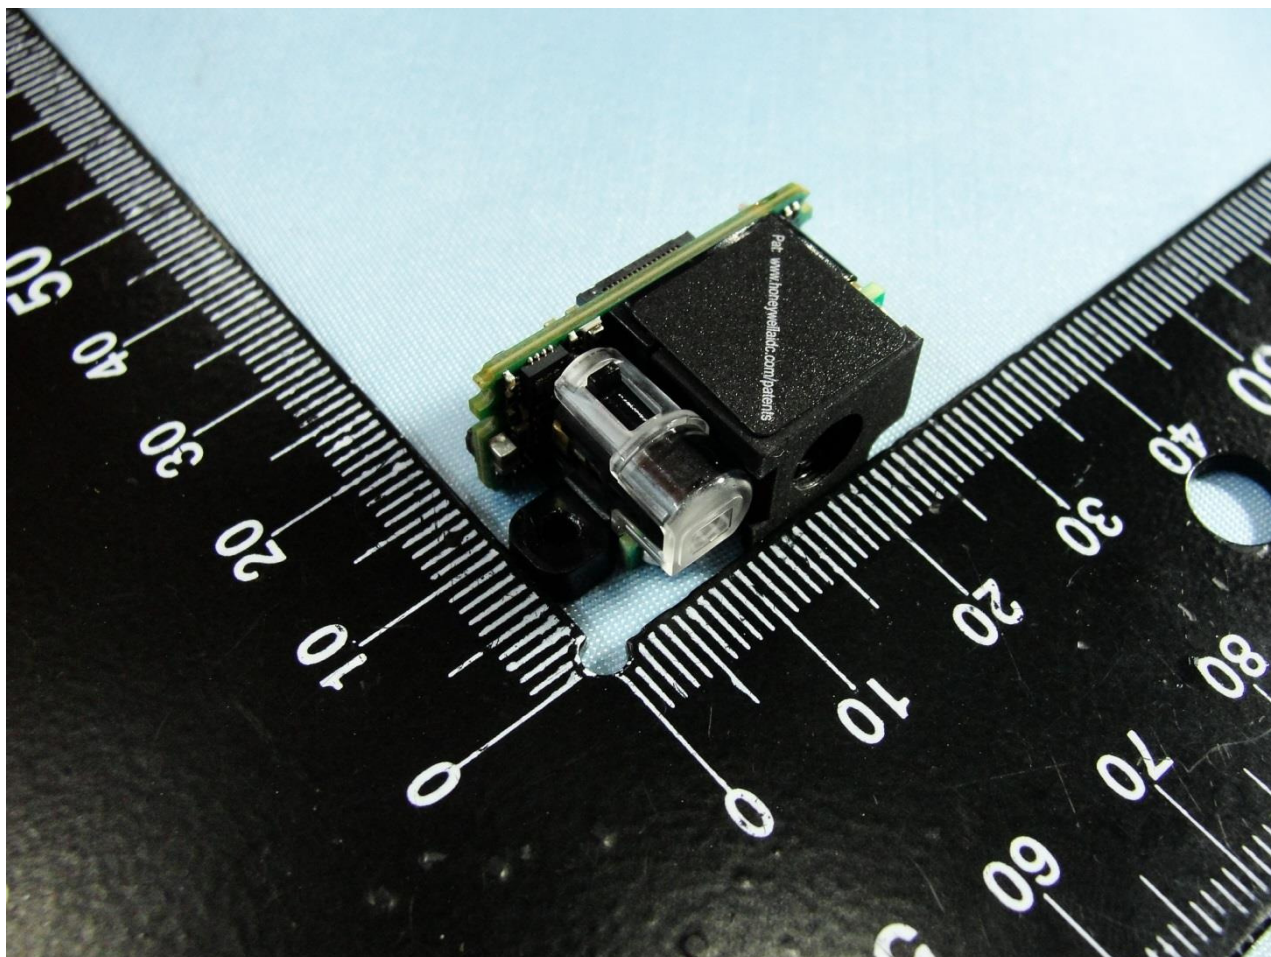


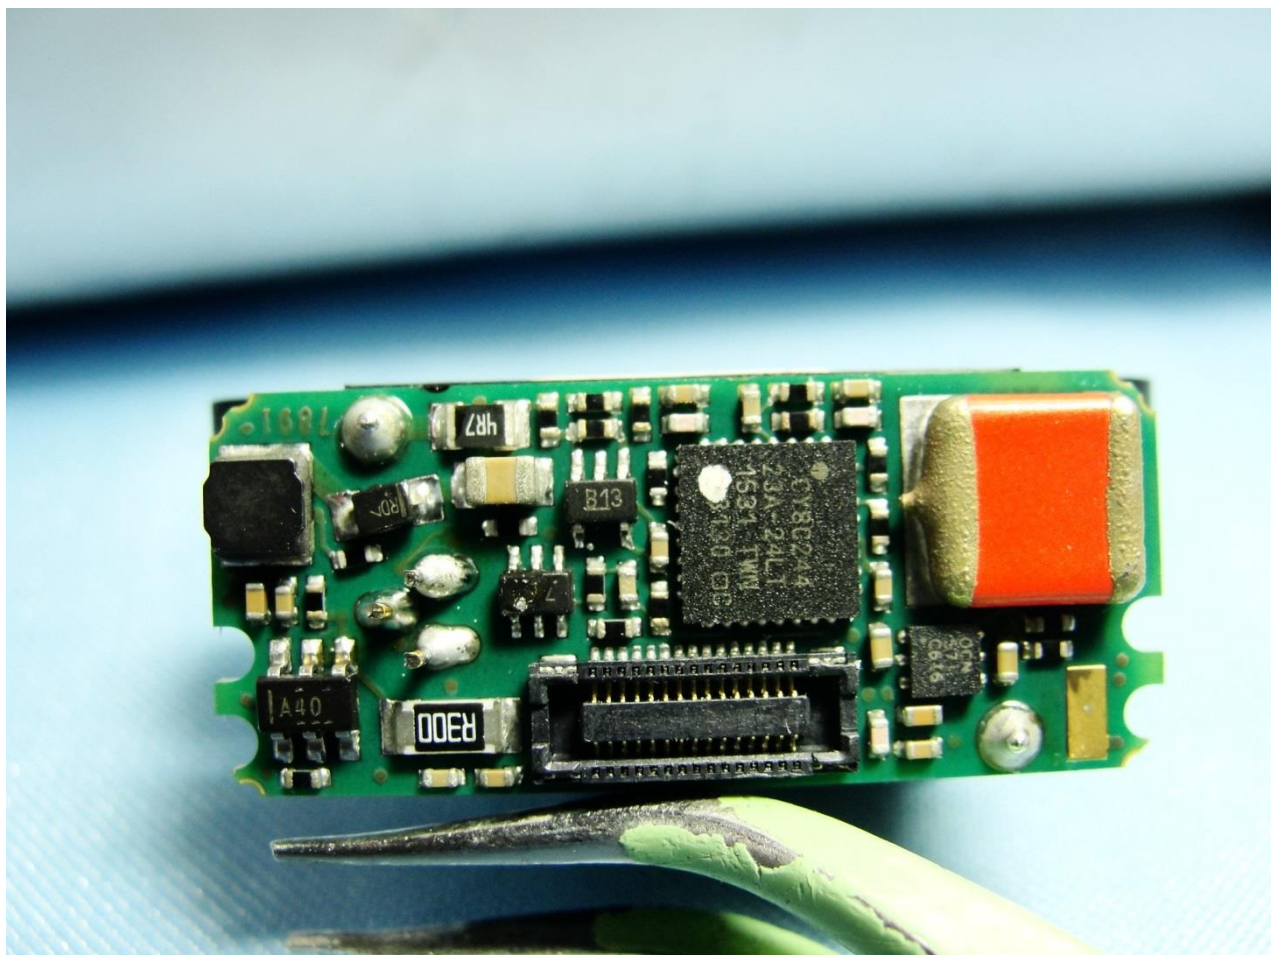**Brand Name: Mio, Mitac, Stryker / Model Name: N450**






Brand Name: Mio, Mitac,Stryker / Model Name: N450

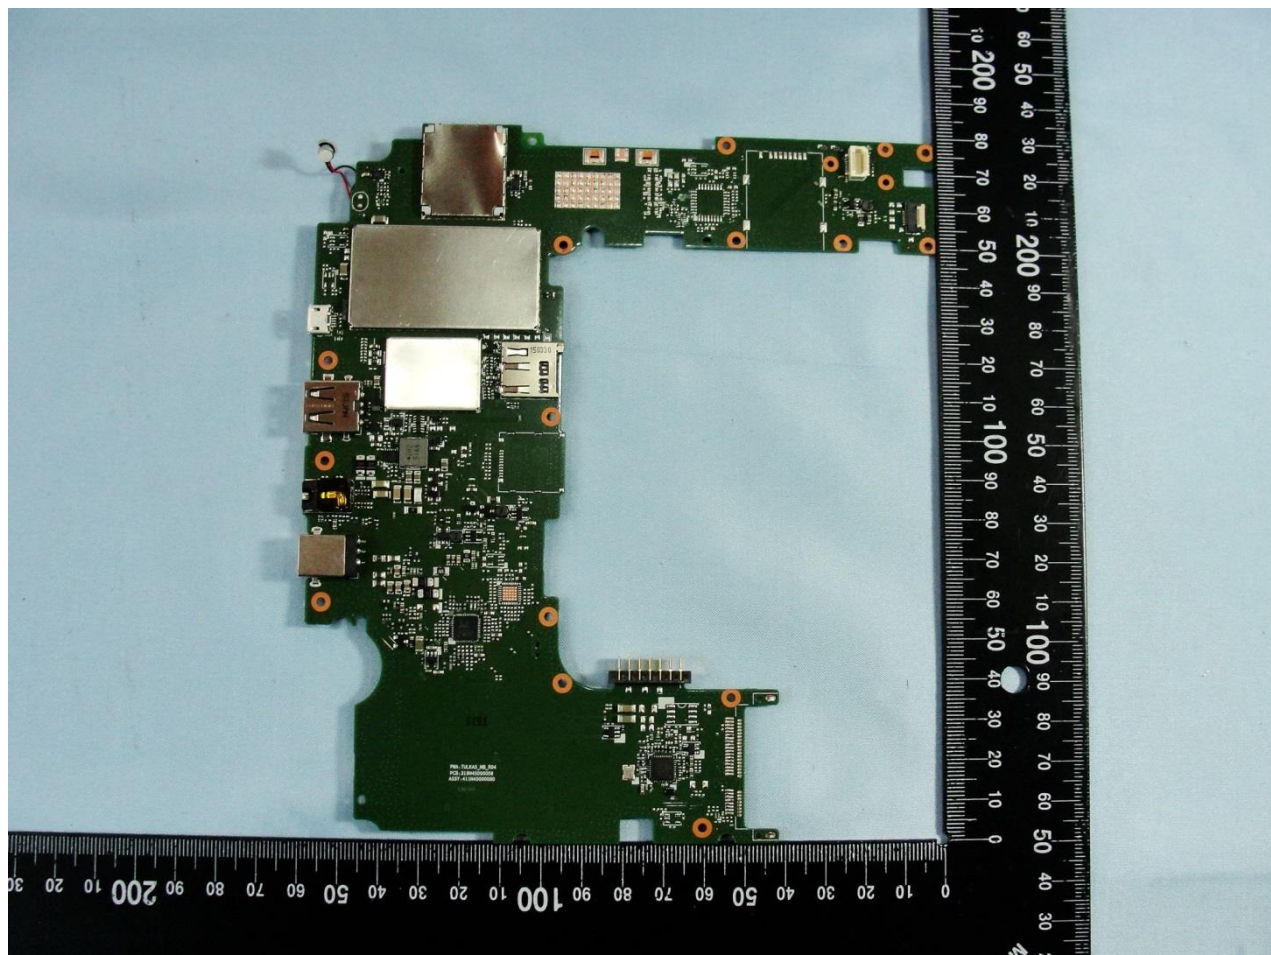


Brand Name: Mio, Mitac,Stryker / Model Name: N450

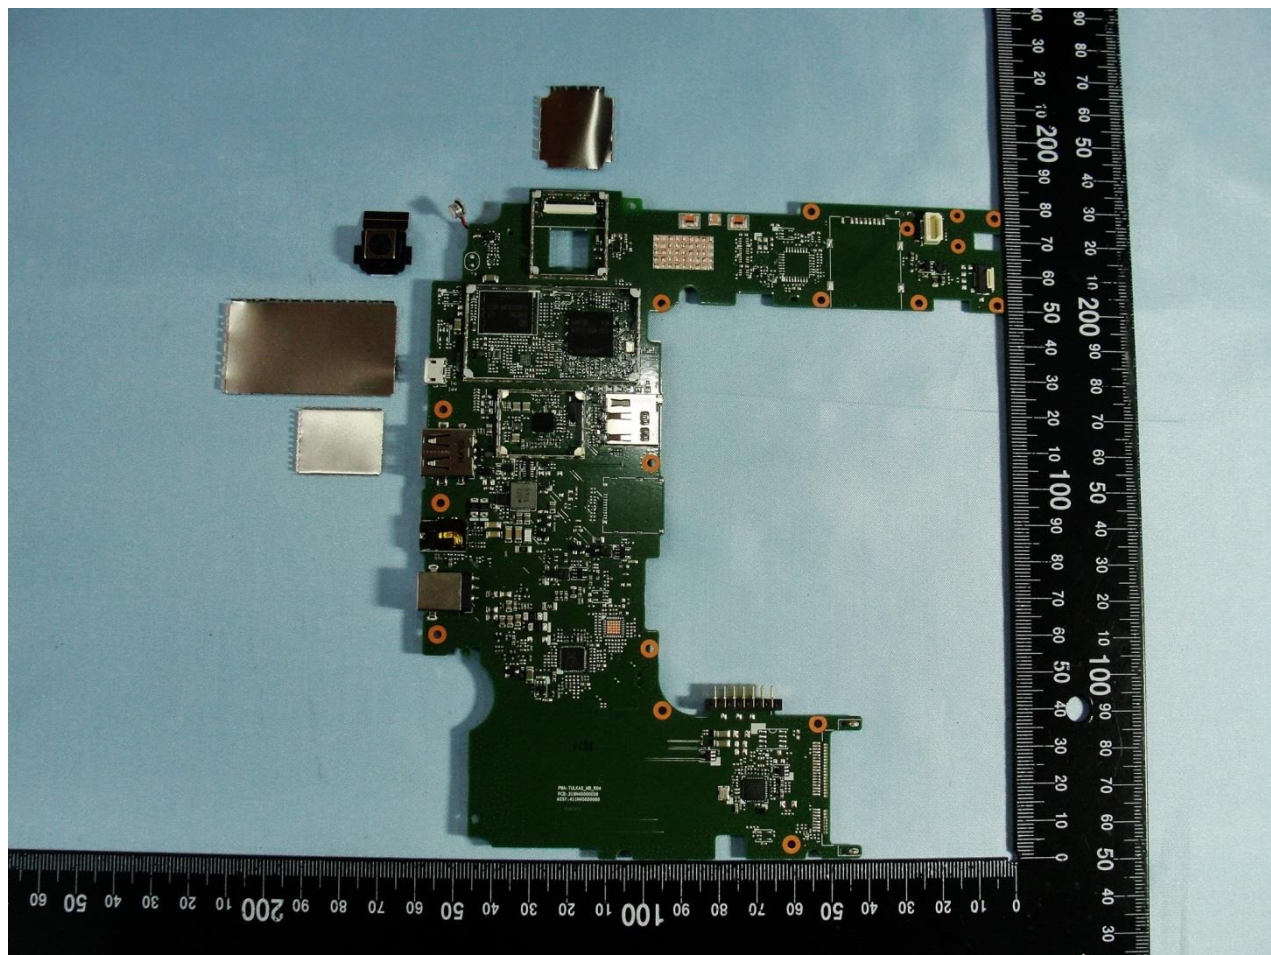




Brand Name: Mio, Mitac, Stryker / Model Name: N450

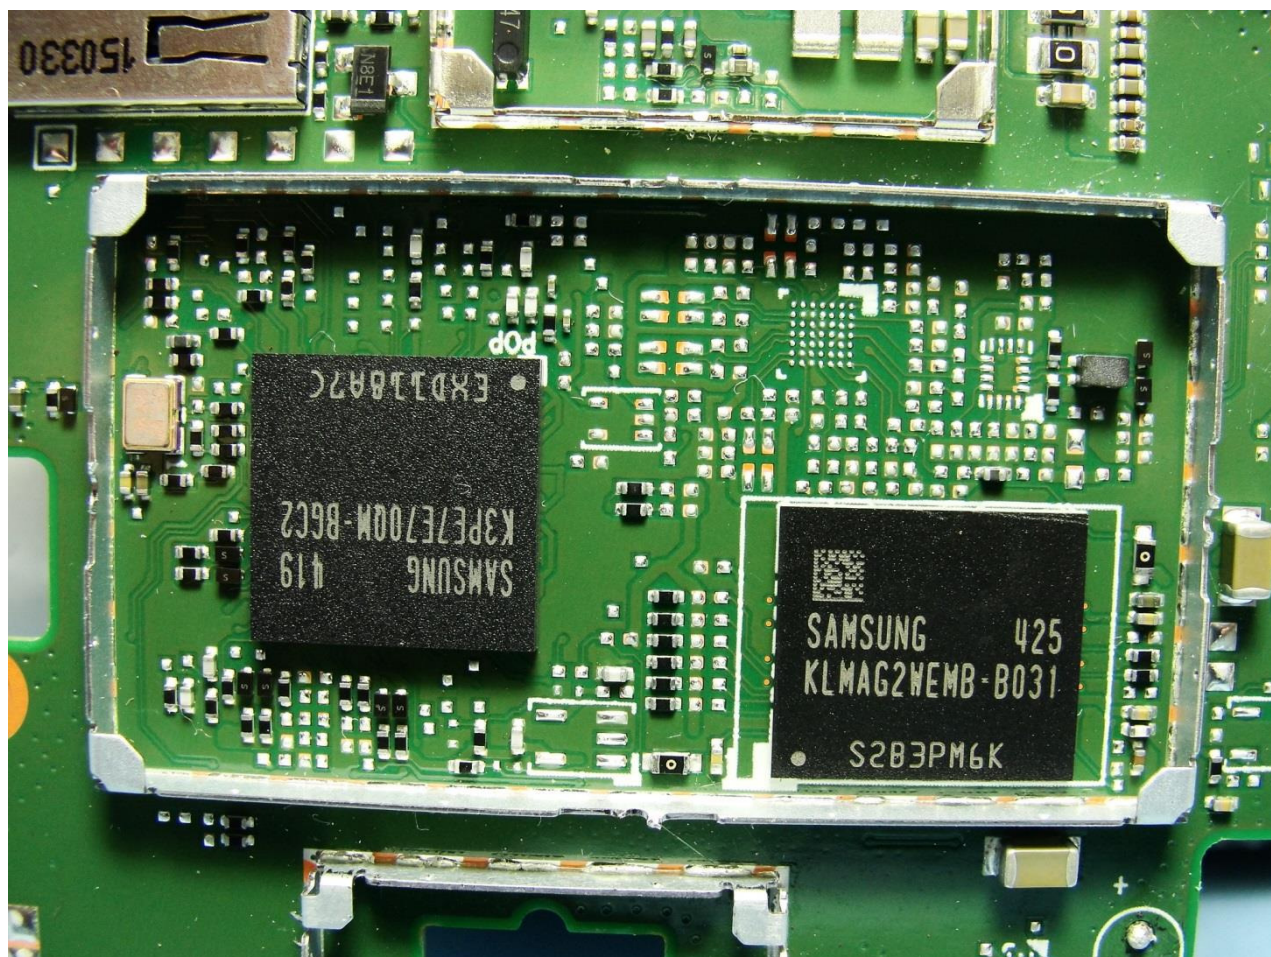

Brand Name: Mio, Mitac, Stryker / Model Name: N450

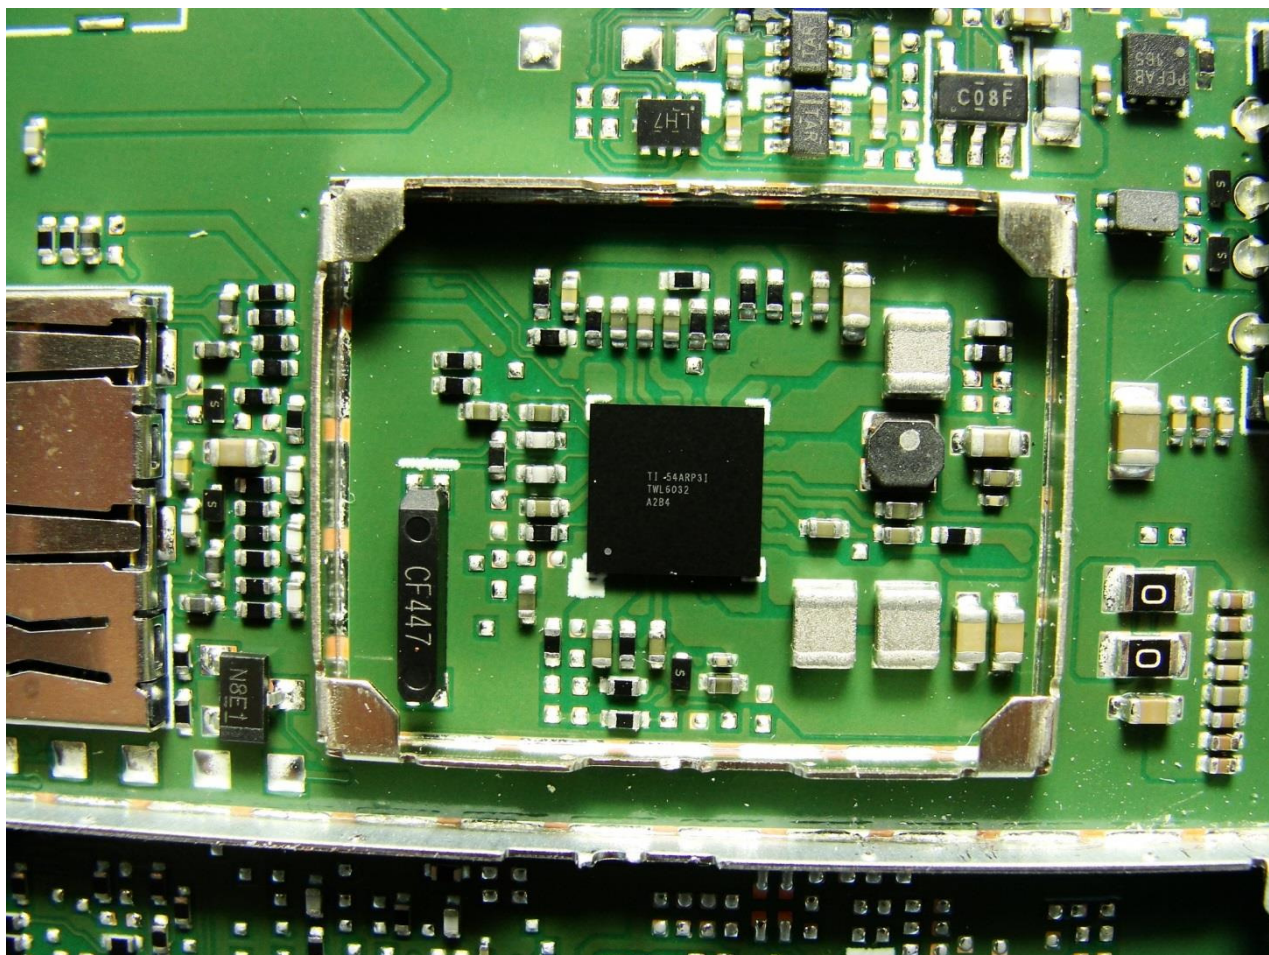





Brand Name: Mio, Mitac, Stryker / Model Name: N450

