TCC

Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



1 (47)

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

FCC HAC Test Report

Test Report Number: WR-905.001

Terminal device: Type: Nokia RM-59, HW: 3101, SW: V MJ100b03.nep (Detailed information is listed in section 5).

Originator: Function: Version/Status: Location:	Anu Balijepalli TCC – Dallas 1.0 Approved TCC Directories
Location:	
Date:	07 September 2005

Change History:

Versior	n Date	Status	Handled By	Comments
0.1	07 September 05	Draft	Anu Balijepalli	Initial Draft
0.2	07 September 05	Review	Anu Balijepalli	Submit for Approval
1.0	07 September 05	Approved	Nerina Walton	Approved

Testing laboratory:	Test & Certification Center (TCC) Dallas Nokia Inc 6021 Connection Drive Irving, Texas 75039 U.S.A.	Client:	Nokia SanDeigo 12278 Scripps Summit Drive San Deigo, California, 92131 U.S.A. Tel. 858-831-5000 Fax. 858-831-6500
	Tel. 972-894-5000 Fax. 972-894-4988		Fax. 000-031-0000

Date and signatures: 07 September 2005 For the Contents: Annadha Anu Balijepalli, Nerina Walton,

Technical Review

Manager Review



Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



2 (47)

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

TABLE OF CONTENTS

1. G	ENERAL	3
1.1 1.2	Objective Test Summary	
	IST OF ABBREVIATIONS, ACRONYMS AND TERMS	
2.1 2.2 2.3	Abbreviations Acronyms Terms	4 4
3. S	TANDARDS BASIS	5
4. T	EST EQUIPMENT LIST	5
5. E	QUIPMENT-UNDER-TEST (EUT)	6
5.1 5.2	DESCRIPTION OF TESTED DEVICE(S): Photograph of Tested Device(S):	
6. T	EST METHOD(S) AND SETUP(S)	7
6.1 6.2 6.3	PROBE DESCRIPTION SPEAG ROBOTIC SYSTEM TEST SETUP	12
7. P	ASS/FAIL CRITERIA	14
8. T	EST PROCEDURE	15
9. S	YSTEM VALIDATION	16
10.	DETAILED TEST RESULTS	25
10.1 10	NEAR FIELD E AND H RF EMISSIONS MEASUREMENTS	
11.	MEASUREMENT UNCERTAINTY	28
APPE	NDIX A: VALIDATIONS SCANS	29
APPE	NDIX B: MEASUREMENT SCANS	34
APPE	NDIX C: PROBE CALIBRATION REPORTS AND DIPOLE CALIBRATION REPORTS	47

© No part of this report shall be reproduced out of the context of the report without the written approval of Nokia Mobile Phones, Inc., Dallas Product Creation, TCC – Dallas.



Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

1. GENERAL

1.1 Objective

This test is performed to ensure that the EUT meets the requirements required by the FCC Method of Measurement for near field E and H emissions. Please note that this report is only for near field emissions, not for the T-coil HAC testing.

1.2 Test Summary

Test Results: The test result relates only to those tested devices mentioned in Section 5 of this test report.

Sample #	Test Performed	Reference	Category
1	Near Field Emissions- E field Near Field Emissions- H field	ANSI C63.19	M3

TCC

Company Confidential

07 September 2005

WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01 Ver 1.0

4 (47)

2. LIST OF ABBREVIATIONS, ACRONYMS AND TERMS

2.1 Abbreviations

dB - decibel

- dBm decibels per milliwatt (absolute measurement)
- MHz megahertz or 1000000 Hertz
- V/m Volts per meter
- A/m Amps per meter

2.2 Acronyms

AMPS - Advanced Mobile Phone System BSS - Base Station Simulator CDMA - Code Division Multiple Access ESN - Electronic Serial Number EUT - Equipment under Test GSM - Global System for Mobile communications IMEI - International Mobile Equipment Identity PCS - Personal Communication System RF- Radio Frequency TDMA - Time Division Multiple Access

2.3 Terms

Base Station Simulator (BSS) - simulates all the necessary signals that a phone would experience while on a live network. There are many types of base station simulators catering for all current protocols, i.e., GSM, AMPS, TDMA, and CDMA.

Cellular - refers to a frequency in the 800MHz band.

PCS - refers to a frequency in the 1900MHz band.

Crest Factor - is the relation between the peak power and the average power in a signal.



07 September 2005

WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

3. STANDARDS BASIS

Testing has been carried out in accordance with:

REF.	Code of the standard	Name of the standard
1	-	ANSI C63.19

Note: Unless otherwise stated, (by reference to a version number and a publication date), the latest version of the above documents applies.

Deviations:

Not Applicable.

4. TEST EQUIPMENT LIST

The listing below indicates the test equipment utilized for the test (s). Calibration interval on all items listed can be obtained from the Engineering Services Group within NMP, Product Creation - Dallas. Where relevant, measuring equipment is subjected to in-service checks between testing. TCC - Dallas shall notify clients promptly, in writing, of identification of defective measuring equipment that casts doubt on the validity of results given in this report.

Test Equipment	NMP #	Calibration Interval	Calibratrion Expiry
SPEAG DASY4 Robot System	2056	NA	NA
SPEAG Data Acquisition Electronics (DAE)	2292	12 months	Jan - 2006
SPEAG E-field Probe ER3DV6	4036	12 months	Jan - 2006
SPEAG H-field Probe H3DV6	4037	12 months	Feb-2006
SPEAG 835MHz Dipole CD835V3	4050	12 months	Apr-2006
SPEAG 1880MHz Dipole CD1880V3	4049	12 months	Jun-2006
Signal Generator HP8648C	0409	12 months	Sep-2005
Boonton Powermeter 4232A	0147	12 months	Sep-2005
AR Power Amplifier 5S1G4	0188	NA	NA
R&S CMU 200	2625	12 months	Nov-2005
R&S FSP	3459	12 months	Jan-2006

5 (47)

Ver 1.0



WR-905.001



Test & Certification Center (TCC) - Dallas

07 September 2005

Accredited Laboratory Certificate Number: 1819-01

5. EQUIPMENT-UNDER-TEST (EUT)

The results in this report relate only to the items listed below:

5.1 Description of Tested Device(s):

Sample #	Mode of Operation	Date of Receipt	Condition of Sample	ltem	Identifying Information
					Type: RM-59
					Model: 6155i
1	CDMA	29 August	Good	Phone	ESN: 044/13202955
	800/1900	2005			HW: 3101
	RC2, SO9				SW: V MJ100b03.nep
					Code: 0522412EM31EZ
					FCC ID: QMNRM-59

5.2 Photograph of Tested Device(s):





6 (47)

Ver 1.0



WR-905.001

07 September 2005



Ver 1.0

7 (47)

Accredited Laboratory Certificate Number: 1819-01

6. TEST METHOD(S) AND SETUP(S)

Test & Certification Center (TCC) - Dallas

Testing was performed in accordance with ANSI C63.19.

6.1 Probe Description

E field Probe Description

Construction

One dipole parallel, two dipoles normal to probe axis

Built-in shielding against static charges Calibration In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%, k=2) Frequency 100 MHz to > 6 GHz; Linearity: ± 0.2 dB (100 MHz to 3 GHz) Directivity ± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis) **Dynamic Range** 2 V/m to > 1000 V/m; Linearity: ± 0.2 dB Dimensions Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm Application General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms

H field Probe Description

Construction

Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges Frequency 200 MHz to 3 GHz (absolute accuracy ± 6.0%, k=2); Output linearized Directivity ± 0.25 dB (spherical isotropy error) **Dynamic Range** 10 mA/m to 2 A/m at 1 GHz **E-Field Interference** < 10% at 3 GHz (for plane wave) Dimensions Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm) Distance from probe tip to dipole centers: 3 mm Application General magnetic near-field measurements up to 3 GHz







WR-905.001

07 September 2005



Ver 1.0

8 (47)

Accredited Laboratory Certificate Number: 1819-01


Field component measurements Surface current measurements Measurements in air or liquids Low interaction with the measured field

Probe Tip Description

Test & Certification Center (TCC) - Dallas


HAC field measurements take place in the close near field with high gradients. Increasing the measuring distance from the source will generally decrease the measured field values. Magnetic field sensors are measuring the integral of the H-field across their sensor area surrounded by the loop. They are calibrated in precise, homogenous field. When measuring a gradient field, the result will be very close to the field in the center of the loop, which is equivalent to the center value. But it will be different from the field at the border of the loop.

Consequently, two sensors with different loop diameters – both calibrated ideally – would give different results when measuring from the edge of the probe sensor elements. The behaviour for electrically small E-field sensors is equivalent. See below for distance plots from a WD, which show the conservative nature of field readings at the probe element center vs. measurements at the sensor end.

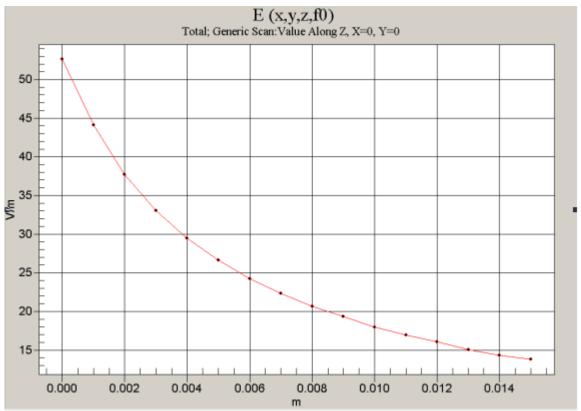

The magnetic field loops of the H3D probes are concentric, with the center 3mm from the tip for H3DV6. Their radius is 1.9mm.

The electric field probes have a more irregular intenal geometry because it is physically not possible to have the 3 orthogonal sensors situated with the same center. The effect of the different sensor centers is accounted for in the HAC uncertainty budget. Their geometric center is at 2.5mm from the tip, and the element ends are 1.1mm closer to the tip.

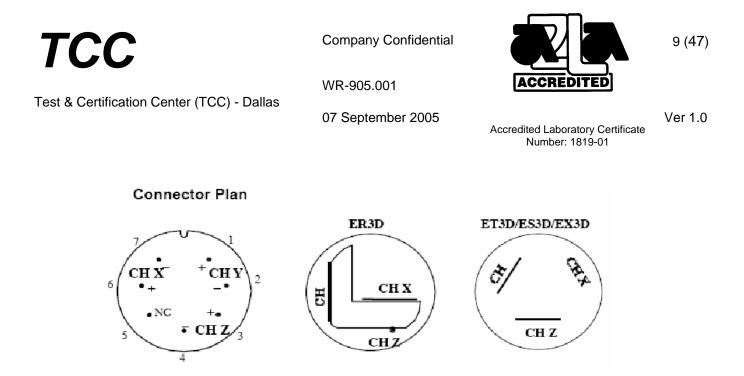

The antistatic shielding inside the probe is connected to the probe connector case. It is recommended to connect the probes with the amplifier using a short and well-shielded cable and to connect the cable shielding with the connector case.

Instrumentation Chain:

Conversion of Connector Voltage to E field

$$E_{i} = \sqrt{\frac{u_{i} + (u_{i}^{2}.CF)/(DCP)}{Norm_{i}.ConvF}}$$

whereby

 E_i = Electric field in V/m

 u_i = Voltage of channel i at the connector in μ V

*Norm*_{*i*} = Sensitivity of channel in $\mu V / (V / m)^2$

ConvF = enhancement factor in liquid (ConvF = 1 for Air)

DCP = Diode compression point in μ V

CF = Signal Crest Factor (peak power/average power)

Probe Response to Frequency

The E-field sensors have inherently a very flat frequency response. They are calibrated with a number of frequencies resulting in a common calibration factor, with the frequency behaviour documented in the calibration certificate.

TCC

Company Confidential



10 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas


WR-905.001

07 September 2005

Accredited Laboratory Certificate Number: 1819-01


Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide R22)



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

H-fileld sensors have frequency dependant sensitivity, which is evaluated for a series of frequencies also visible in the probe calibration certificate. The calibration factors result from a fitting algorithm. The proper conversion is calculated by the DASY4 software depending on the frequency setting in the procedure.

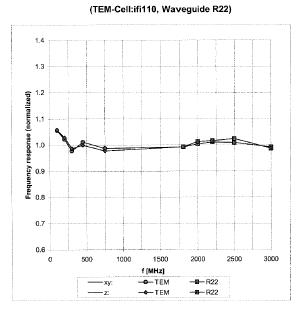

Frequency Response of H-Field

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)



WR-905.001

07 September 2005



Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

Conversion to Peak

Test & Certification Center (TCC) - Dallas

Peak is defined as Peak Envelope Power. All raw measurements from the HAC measurement system are RMS values. The DASY4 system incorporates the crest factor of the signal in the computation of the RMS values. Although the software also has capability to estimate the peak field by applying a square root of crest factor value to the readings, the probe modulation factor was applied manually instead per PC63.19 in the measurement tables in this report. The equation to convert the raw measurements in the data tables are:

Peak Field = 20 log (Raw x PMF)

Where:


Peak Field = Peak field (in dBV/m or dBA/m)

Raw = Raw field measurement from the measurement system (in V/m or A/m).

PMF = Probe Modualtion Factor (in linear units).



WR-905.001





Ver 1.0

Number: 1819-01


Accredited Laboratory Certificate

6.2 Speag Robotic System

Test & Certification Center (TCC) - Dallas

E-field and H-field measurements are performed using the DASY4 automated dosimetric assessment system. The DASY4 is made by Schmid & Partner Engineering AG (SPEAG) and consists of high precision robotics system (Staubli), robot controller. Pentium 4 computer, near- field probe, probe alignment sensor, and the HAC phantom. The robot is a six- axis industrial robot performing precise movements to the position the probe to the location of maximum EMF.

System Hardware

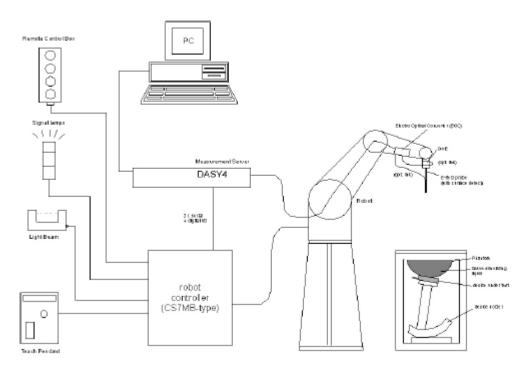

A cell controller system contains the power supply, robot controller; teach pendant, and a remote control used to drive the robot motors. The PC consists of RF meaurement system DASY4 V4.5 with HAC extension, A/D interface card, monitor, mouse and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD conversion, offset measurements, mechanical surface detection, collision detection, etc is connected to the Electro - optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

The DAE consists of a highly sensitive electrometer – grade preamplifier with auto-zeroing, a channel and gain switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe-mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built- in VME-bus computer.



WR-905.001

07 September 2005



Ver 1.0

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Data Evaluation

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_2 * (cf/dcpi)$$

with V_i = compensated signal of channel i (i = x, y, z)

 U_i = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter) dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:
$$E_i = \sqrt{\frac{V_i}{Norm_i x ConvF}}$$

H-field probes:
$$H_i = \sqrt{V_i} x \frac{a_{io} + a_{i1}f + a_{i2}f^2}{f}$$

with $V_i = \text{compensated signal of channel i } (i = x, y, z)$ $Norm_i = \text{sensor sensitivity of channel i } (i = x, y, z)$ $\mu V/(V/m)_2 \text{ for E-field Probes}$ ConvF = sensitivity enhancement in solution $a_{ij} = \text{sensor sensitivity factors for H-field probes}$ f = carrier frequency [GHz] $E_i = \text{electric field strength of channel i in V/m}$ $H_i = \text{magnetic field strength of channel i in A/m}$

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

TCC

Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

14 (47)

6.3 Test Setup

The test setup is shown in the picture below.



7. PASS/FAIL CRITERIA

The EUT must meet the following M3 category standards -

Category	1	Wireless Device Parameters				
Near field	AWF	E-field Emissions	H-field Emissions			
		Peak – V/m	Peak – A/m			
Category M3	AWF =0 (TDMA, CDMA)	63.1 to 112.2	0.19 to 0.34			
	AWF = -5 (GSM)	47.3 to 84.1	0.15 to 0.25			
Category M4	AWF =0 (TDMA, CDMA)	< 63.1	< 0.19			
	AWF = -5 (GSM)	< 47.3	< 0.15			



WR-905.001

07 September 2005



Ver 1.0

Accredited Laboratory Certificate Number: 1819-01


8. TEST PROCEDURE

Test & Certification Center (TCC) - Dallas

The following illustrates a typical RF emissions test scan over a wireless communication device:

- Proper operation of the field probe, probe measurement system, other instrumentation, and the positioning system was confirmed.
- WD is positioned in its intended test position, acoustic output point of the device perpendicular to the field probe.
- The WD operation for maximum rated RF output power was configured and confirmed with the base station simulator, at the test channel and other normal operating parameters as intended for the test. The battery was ensured to be fully charged before each test.
- The center sub-grid was centered over the center of the acoustic output (also audio band magnetic output, if applicable). The WD audio outout was positioned tangent (as physically possible) to the measurement plane.
- The measurement system measured the field strength at the reference location.
- Measurements at 2mm increments in the 5x5 cm region were performed and recorded. A 360 deg rotation about the azimuth axis at the maximum interpolated position was measured. For the worst case condition, the peak reading from this rotation was used in re-evaluating the HAC category.
- The system performed a drift evaluation by measuring the field at the reference location.
- Same steps were done for both the E and H field measurements.







WR-905.001

07 September 2005



Ver 1.0

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01


9. SYSTEM VALIDATION

The input signal was an unmodulated continous wave. The following points were taken into consideration in performing the system validation:

Average Input Power = 100mW (20dBm RMS) after adjustment for return loss.

The test fixture must meet the 2-wavelength separation criterion.

The proper measurement of the 1cm probe to dipole separation, which is measured from the top surface of the dipole to the calibration reference point of the sensor, defined by the probe manufacturer is shown in the following picture:

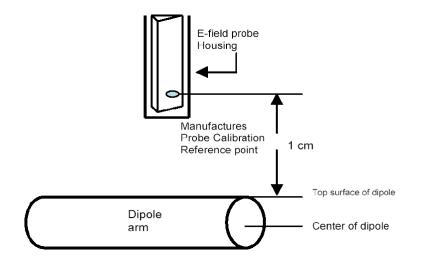

To assure proper operation of the near-field measurement probe the input power to the dipole shall be commensurate to with the full rated output power of the wireless device (eg. – for a cellular phone wireless device the average peak antenna input power will be on the order of 100mW (ie, 20dBm) RMS after adjustment for any mismatch.

A dipole antenna meeting the requirements in PC63.19 was placed in the position normally occupied by the WD. The length of the dipole was scanned with both E-field and H-field probes and the maximum values for each were recoreded.

Using the near-field measurement system, scan the antenna over the radiating dipole and record the greatest field reading observed. Due to the nature of E-fields about freespace dipoles, the two E-field peaks measured over the dipole are averaged to compensate for non-paralellity of the setup, See manufacturer method on dipole calibration certificates, page 2. Field strength measurements shall be made only when the probe is stationary.






Test & Certification Center (TCC) - Dallas

WR-905.001

07 September 2005

Ver 1.0 Accredited Laboratory Certificate Number: 1819-01

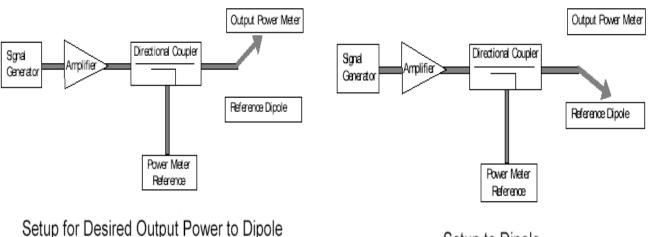


Setup to Dipole

Using this setup configuration, the signal generator was adjusted for the desired output power (100mW) at a specified frequency. The reference power from the coupled port of the directional coupler is recorded. Next, the output cable is connected to the reference dipole, as shown in the figure above.

The input signal was adjusted until the reference power from the coupled port of the directional coupler was the same as previously recorded, to compensate for the impendance mismatch between the output cable and the reference dipole.

To assure proper operation of the near-field measurement probe the input power to the reference dipole was verified to the full rated output power of the wireless device. The dipole was secured in a holder in a manner to meet the 20dB reflection. The near-field measurement probe was positioned over the dipole.

The antenna was scanned over the appropriate sized area to cover the dipole from end to end. SPEAG uses 2D interpolation algorithms between the measured points. Please see below two-dimensional plots showing that the interpolated values interpolate smoothly between 5mm steps for a free space RF dipole:

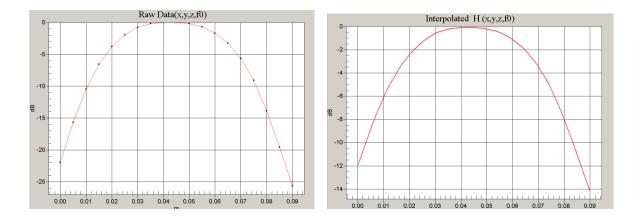



07 September 2005

WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate

Ver 1.0

18 (47)

Number: 1819-01

Validations were performed for CW at 20dBm peak power.

		Recorded	Target Value	% deviation
	E field	154.0	162.1	5.00%
835 MHz	H field	0.422	0.451	6.43%
	E field	129.1	137.6	6.18%
1880 MHz	H field	0.424	0.452	6.19%

Note: Please see Appendix A for the Validation Scans



WR-905.001

07 September 2005



Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

MODULATION FACTOR

Test & Certification Center (TCC) - Dallas

A calibration was made of the modulation response of the probe and its instrumentation chain. This calibration was performed with the field probe, attached to its instrumentation. The response of the probe system to a CW field at the frequency of interest is compared to its response to a modulated signal with equal peak amplitude to that of a CW signal. The field level of the test signals are ensured to be more than 10dB above the ambient level and the noise floor of the instrumentation being used. The ratio of the CW reading to that taken with a modulated reading was applied to the DUT measurements.

This was done using the following procedure:

- The probe was illuminated with a CW signal at the intended measurement frequency.
- The probe was positioned at the field maxima over the dipole antenna (determined afer an area scan over the dipole).
- The reading of the probe measurement system of the CW signal at the maximum point was recorded.
- Using a Spectrum Analyzer, the modulated signal adjusted with the same peak level of the CW signal was determined.
- The probe measurement system reading was recorded with the modulated signal.
- The ratio of the CW reading to the modulated signal reading is the probe modulation factor (PMF) for the modulation and field probe combination.
- Same steps are repeated at all frequency bands and for both E and H field probes.

The modulation factors obtained were applied to readings taken of the actual wireless device, in order to obtain an accurate peak field reading using the formula:

Peak = 20log(Raw x PMF)

This method correlates well with the modulation using the DUT in the alternative substitution method. See below for correlation of signal:



WR-905.001




Test & Certification Center (TCC) - Dallas


07 September 2005

Accredited Laboratory Certificate Number: 1819-01

Signal Generator Modulated Signal:

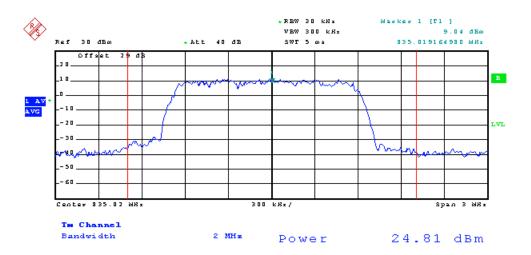

Wireless Device Modulated Signal:

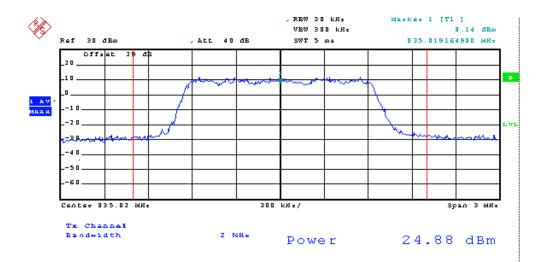

20 (47)

Ver 1.0



WR-905.001





Test & Certification Center (TCC) - Dallas


07 September 2005

Ver 1.0 Accredited Laboratory Certificate Number: 1819-01

Modulation Factors were performed for CW, 80%AM and the modulated signal at 20dBm peak power, See below for the picture as well as the Spectrum Analyzer Plots.

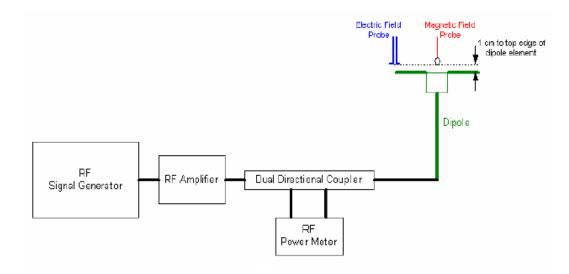



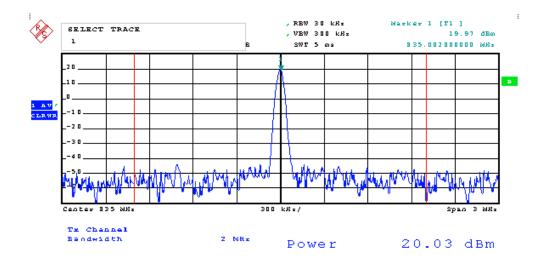

CW Signal for 850MHz band





Test & Certification Center (TCC) - Dallas


WR-905.001

07 September 2005


Ver 1.0

22 (47)

Accredited Laboratory Certificate Number: 1819-01

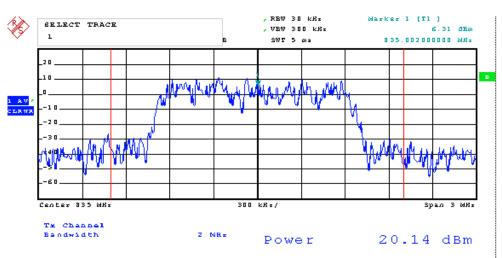

CDMA Signal for 850MHz band

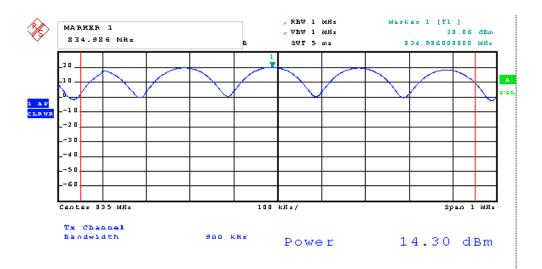

80%AM Signal for 850MHz band





Test & Certification Center (TCC) - Dallas


WR-905.001

07 September 2005


Ver 1.0

23 (47)

Accredited Laboratory Certificate Number: 1819-01

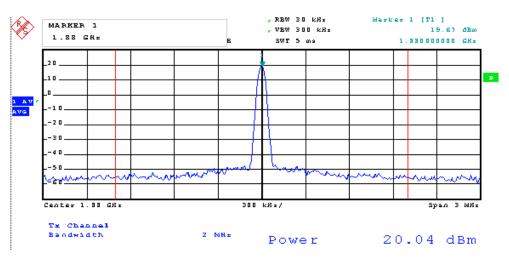

CW Signal for 1900MHz band

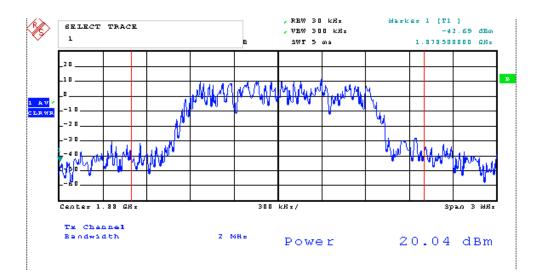

CDMA Signal for 1900MHz band






Test & Certification Center (TCC) - Dallas

WR-905.001

07 September 2005

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

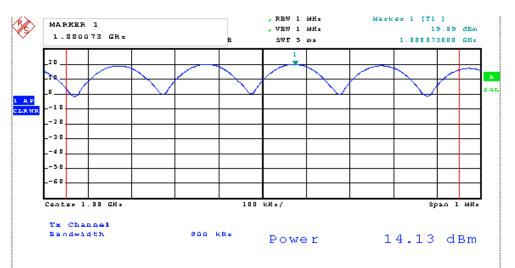

80%AM Signal for 1900MHz band

835 MHz	E-Field	H-Field	Modulation Factor (MF) for	Modulation Factor (MF) for
	(V/m)	(A/m)	E-field	H-field
CDMA	152.2	0.43	1.0	1.0
CW	152.0	0.41		
80%AM	90.3	0.25		

1880 MHz	E-Field	H-Field	Modulation Factor (MF) for	Modulation Factor (MF) for
	(V/m)	(A/m)	E-field	H-field
CDMA	118.3	0.57	1.0	0.7
CW	115.0	0.38		
80%AM	71.5	0.24		

24 (47)



WR-905.001



Test & Certification Center (TCC) - Dallas

07 September 2005

Accredited Laboratory Certificate Number: 1819-01

10. DETAILED TEST RESULTS

Test Technician / Engineer	Anu Balijepalli				
Date of Measurement	August 31-September 2, 2005				
Temperature / Humidity / Pressure	20-25°C	45-60%RH	29-31 in		
Test Result	Complies				

10.1 Near Field E and H RF emissions measurements

10.1.1 Test Results

Note: Testing was done at the antenna extended position. See Appendix B for the grids and plots of these cases.

CDMA CELLULAR E - FIELD

CDMA Celluar	Conducted Power	Power Drift	E (V/m)	Modulation Factor	Peak Field	Excluded Blocks
	(dBm)	(dB)			(V/m)	
Ch 1013	25.0	0.107	70.3	1.0	70.3	1,2,4
Ch 384	25.0	0.0996	77.2	1.0	77.2	1,2,4
Ch 777	25.0	0.119	66.7	1.0	66.7	1,2,4

CDMA CELLULAR H- FIELD

CDMA Celluar	Conducted Power	Power Drift	H (A/m)	Modulation Factor	Peak Field	Excluded Blocks
	(dBm)	(dB)			(A/m)	
Ch 1013	25.0	-0.0131	0.115	1.0	0.115	7,8,9
Ch 384	25.0	-0.111	0.122	1.0	0.122	7,8,9
Ch 777	25.0	-0.0673	0.109	1.0	0.109	7,8,9

25 (47)

Ver 1.0



WR-905.001



26 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas

07 September 2005

Accredited Laboratory Certificate Number: 1819-01

CDMA PCS E - FIELD

CDMA PCS	Conducted Power (dBm)	Power Drift (dB)	E (V/m)	Modulation Factor	Peak Field (V/m)	Excluded Blocks
Ch 25	23.1	-0.0184	27.1	1.0	27.1	1,4,7
Ch 600	23.2	0.298	29.5	1.0	29.5	1,4,7
Ch 1175	23.1	0.0551	30.5	1.0	30.5	1,4,7

CDMA PCS H - FIELD

CDMA PCS	Conducted Power	Power Drift	H (A/m)	Modulation Factor	Peak Field	Excluded Blocks
	(dBm)	(dB)			(A/m)	
Ch 25	23.1	0.174	0.071	0.7	0.0497	7,8,9
Ch 600	23.2	-0.214	0.081	0.7	0.0567	7,8,9
Ch 1175	23.1	-0.0628	0.080	0.7	0.0560	6,8,9



WR-905.001



Test & Certification Center (TCC) - Dallas

07 September 2005

Accredited Laboratory Certificate Number: 1819-01


Ver 1.0

27 (47)

WORST CASE CONFIGURATION

CDMA Celluar	E (V/m)	Modulation Factor	Peak Field (V/m)	FCC M3 Limits (V/m)	Category
Ch 384	78.0	1.0	78.0	63.1 to 112.2	M3

The probe rotation was done at the sub grid 7 for Channel 384, E field.

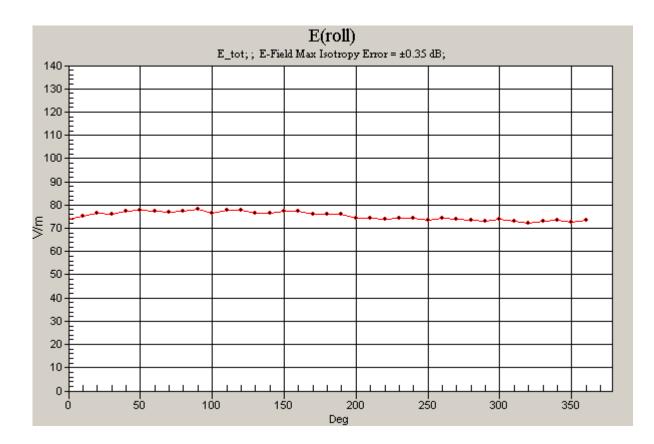

TCC

Company Confidential

WR-905.001

07 September 2005



28 (47)

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

11. MEASUREMENT UNCERTAINTY

Test & Certification Center (TCC) - Dallas

HAC Uncertainty	Budget								
Error Description	Uncertainty value	Prob. Dist.	Div.	(ci) E	(ci) H	Std. Unc. E	Std. Unc. H	Squared E	Squared H
Measurement System									
Probe Calibration	5.1	N	1	1	1	5.1	5.1	26.0	26.0
Axial Isotropy	4.7	R	1.7321	1	1	2.7	2.7	7.4	7.4
Sensor Displacement	16.5	R	1.7321	1	0.145	9.5	1.4	90.7	1.9
Boundary Effects	2.4	R	1.7321	1	1	1.4	1.4	1.9	1.9
Linearity	4.7	R	1.7321	1	1	2.7	2.7	7.4	7.4
Scaling to Peak Envelope Power	2	R	1.7321	1	1	1.2	1.2	1.3	1.3
System Detection Limit	1	R	1.7321	1	1	0.6	0.6	0.3	0.3
Readout Electronics	0.3	N	1	1	1	0.3	0.3	0.1	0.1
Response Time	0.8	R	1.7321	1	1	0.5	0.5	0.2	0.2
Integration Time	2.6	R	1.7321	1	1	1.5	1.5	2.3	2.3
RF Ambient Conditions	3	R	1.7321	1	1	1.7	1.7	3.0	3.0
RF Reflections	12	R	1.7321	1	1	6.9	6.9	48.0	48.0
Probe Positioner	1.2	R	1.7321	1	0.67	0.7	0.5	0.5	0.2
Probe Positioning	4.7	R	1.7321	1	0.67	2.7	1.8	7.4	3.3
Extrap. And Interpolation	1	R	1.7321	1	1	0.6	0.6	0.3	0.3
Test Sample Related								0.0	0.0
Device Positioning Vertical	10	R	1.7321	1	0.67	2.7	1.8	7.4	3.3
Device Positioning Lateral	10	R	1.7321	1	1	0.6	0.6	0.3	0.3
Device Holder	2.4	R	1.7321	1	1	1.4	1.4	1.9	1.9
Power Drift	5	R	1.7321	1	1	2.9	2.9	8.3	8.3
Phantom and Setup Related								0.0	0.0
Phantom Thickness	2.4	R	1.7321	1	0.67	1.4	0.9	1.9	0.9
Combined Std. Ur	ncertainty							16.6	12.8
Expanded Std. Uncerta (k=2)	ainty on Field							33.2%	21.8%



Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



29 (47)

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

APPENDIX A: VALIDATIONS SCANS



WR-905.001

07 September 2005



30 (47)

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

Date/Time: 8/30/2005 1:36:40 PM Test Laboratory: TCC Dallas

835MHz, E field, CW Validation

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.00461 dB

HAC Procedure/Hearing Aid Compatibility Test 0 deg (81x401x1): Measurement grid: dx=5mm, dy=5mm Maximum value of Total field (slot averaged) = 158.1 V/m Hearing Aid Near-Field Category: M2 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

	-			-	
Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
152.9	158.1	129.1	152.9	158.1	129.1
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
75.2	87.6	83.9	75.2	87.6	83.9
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
122.6	149.8	145.6	122.6	149.8	145.6

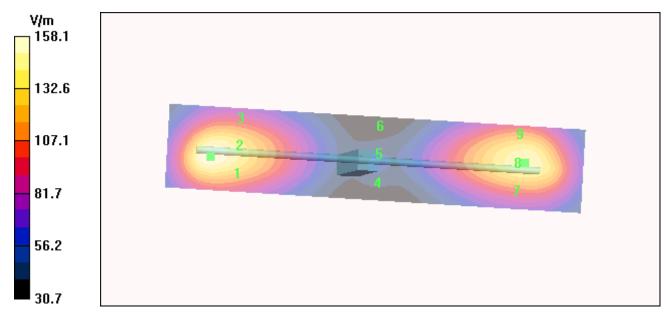

FCC HAC Test Report



WR-905.001

07 September 2005



31 (47)

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01 Ver 1.0

Date/Time: 8/30/2005 2:09:37 PM Test Laboratory: TCC Dallas

835MHz, H field, CW Validation

Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.0274 dB

HAC Procedure/Hearing Aid Compatibility Test 0 deg (81x401x1): Measurement grid: dx=5mm, dy=5mm Maximum value of Total field (slot averaged) = 0.422 A/m Hearing Aid Near-Field Category: M2 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 2 Grid 2 Grid 3 Grid 1 Grid 1 Grid 3 0.299 0.362 0.335 0.299 0.362 0.335 Grid 4 Grid 5 Grid 6 Grid 4 Grid 5 Grid 6 0.353 0.422 0.388 0.353 0.422 0.388 Grid 7 Grid 8 Grid 9 Grid 7 Grid 8 Grid 9 0.307 0.364 0.334 0.307 0.364 0.334

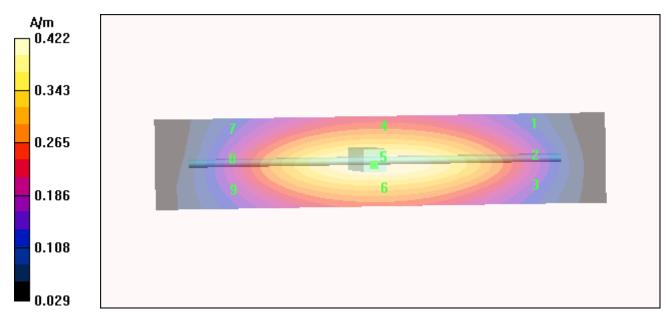

FCC HAC Test Report



WR-905.001

07 September 2005



32 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 8/30/2005 2:57:52 PM Test Laboratory: TCC Dallas

1880MHz, E field, CW Validation

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.0302 dB

HAC Procedure/Hearing Aid Compatibility Test 0 deg (81x181x1): Measurement grid: dx=5mm, dy=5mm Maximum value of Total field (slot averaged) = 130.4 V/mHearing Aid Near-Field Category: M2 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

	۰ ۱	•		٠	•
Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
108.8	127.8	116.5	108.8	127.8	116.5
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
74.6	87.0	83.8	74.6	87.0	83.8
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
107.5	130.4	123.3	107.5	130.4	123.3

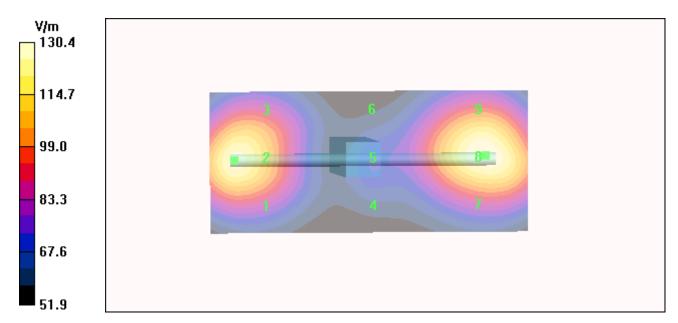

FCC HAC Test Report



WR-905.001

07 September 2005



Ver 1.0

33 (47)

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 8/30/2005 2:43:21 PM Test Laboratory: TCC Dallas

1880MHz, H field, CW Validation

Test & Certification Center (TCC) - Dallas

Communication System: CW; Frequency: 1880 MHz;Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0182 dB

HAC Procedure/Hearing Aid Compatibility Test 0 deg (81x181x1): Measurement grid: dx=5mm, dy=5mm Maximum value of Total field (slot averaged) = 0.424 A/m Hearing Aid Near-Field Category: M2 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 2 Grid 3 Grid 2 Grid 1 Grid 1 Grid 3 0.320 0.388 0.356 0.320 0.388 0.356 Grid 4 Grid 5 Grid 6 Grid 4 Grid 5 Grid 6 0.351 0.424 0.395 0.351 0.424 0.395 Grid 7 Grid 8 Grid 9 Grid 7 Grid 8 Grid 9 0.315 0.384 0.362 0.315 0.384 0.362

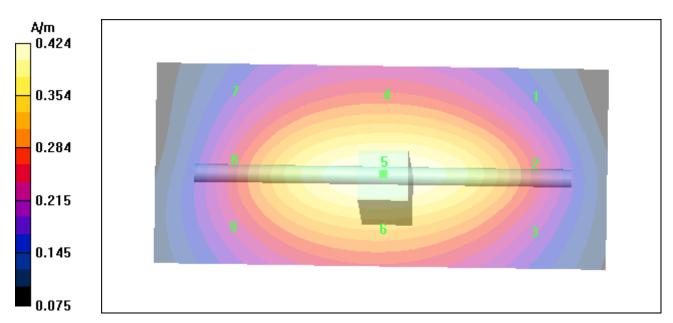

FCC HAC Test Report



Test & Certification Center (TCC) - Dallas

Company Confidential

WR-905.001

07 September 2005



Accredited Laboratory Certificate Number: 1819-01 34 (47)

Ver 1.0

APPENDIX B: MEASUREMENT SCANS



07 September 2005

WR-905.001



35 (47)

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

Date/Time: 8/31/2005 1:36:54 PM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch1013, Whip Extend position, E field

Communication System: CDMA800; Frequency: 824.7 MHz; Duty Cycle: 1:1 **DASY4** Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.107 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 70.3 V/mHearing Aid Near-Field Category: M3 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)


Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
74.0	71.1	56.6	74.0	71.1	56.6
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
70.4	69.7	56.6	70.4	69.7	56.6
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
70.3	67.4	50.6	70.3	67.4	50.6

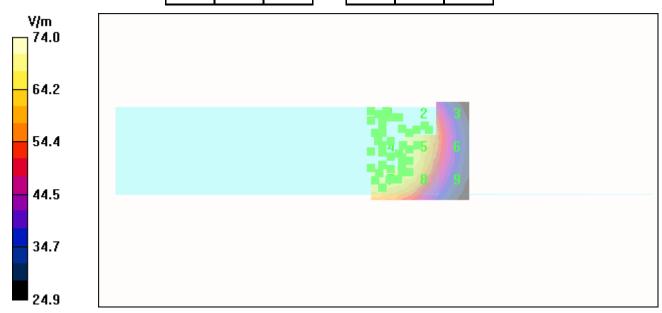



WR-905.001

Test & Certification Center (TCC) - Dallas





36 (47)

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 8/31/2005 1:13:12 PM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch384, Whip Extend position, E field

Communication System: CDMA800; Frequency: 836.52 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.0996 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 77.2 V/m Hearing Aid Near-Field Category: M3 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
83.0	77.9	57.6	83.0	77.9	57.6
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
78.3	75.5	57.5	78.3	75.5	57.5
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
77.2	73.9	51.0	77.2	73.9	51.0

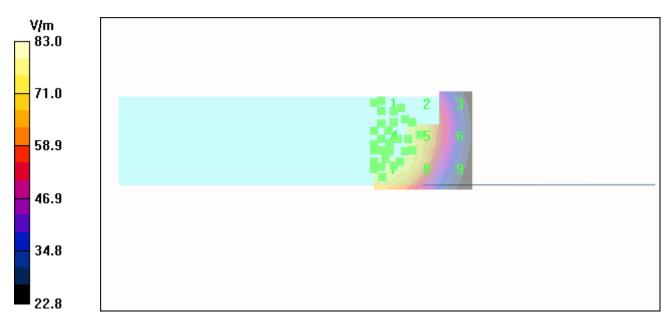



WR-905.001

Test & Certification Center (TCC) - Dallas

07 September 2005



Ver 1.0

37 (47)

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 8/31/2005 1:59:11 PM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch777, Whip Extend position, E field

Communication System: CDMA800; Frequency: 848.31 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.119 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 66.7 V/mHearing Aid Near-Field Category: M3 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
72.9	68.6	52.4	72.9	68.6	52.4
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
67.3	65.2	52.5	67.3	65.2	52.5
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
66.7	62.8	46.1	66.7	62.8	46.1

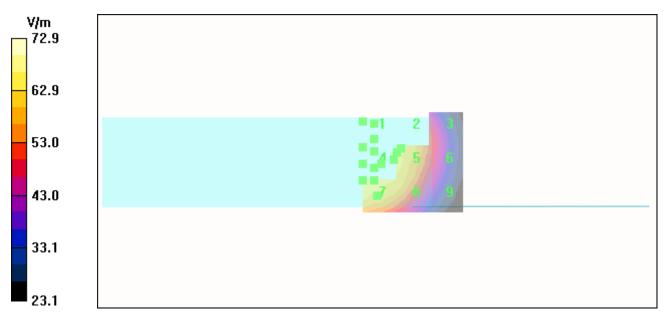



07 September 2005

WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

38 (47)

Date/Time: 9/1/2005 8:54:02 AM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch1013, Whip Extend position, H field

Communication System: CDMA800; Frequency: 824.7 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0131 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.109 A/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged)

H in A/m (Slot averaged) Grid 2 Grid 3 Grid 1 Grid 1 Grid 2 Grid 3 0.095 0.101 0.101 0.095 0.101 0.101 Grid 4 Grid 5 Grid 6 Grid 4 Grid 5 Grid 6 0.094 0.108 0.109 0.094 0.108 0.109 Grid 8 Grid 8 Grid 7 Grid 9 Grid 7 Grid 9 0.127 0.119 0.115 0.127 0.119 0.115

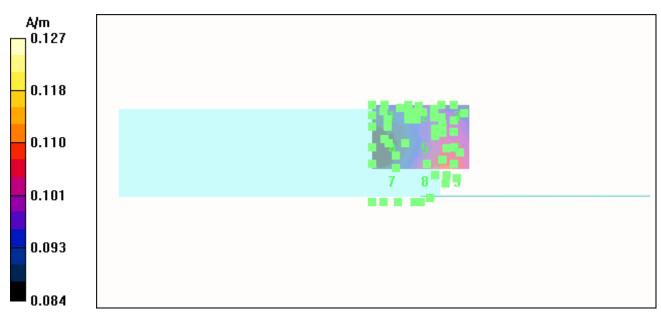



WR-905.001



Accredited Laboratory Certificate Number: 1819-01

39 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas 07 September 2005

Date/Time: 9/1/2005 8:31:42 AM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch384, Whip Extend position, H field

Communication System: CDMA800; Frequency: 836.52 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.111 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.114 A/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

	`	0	<u>.</u>		`	0,
Grid 1	Grid 2	Grid 3		Grid 1	Grid 2	Grid 3
0.095	0.104	0.106		0.095	0.104	0.106
Grid 4	Grid 5	Grid 6		Grid 4	Grid 5	Grid 6
0.094	0.113	0.114		0.094	0.113	0.114
Grid 7	Grid 8	Grid 9		Grid 7	Grid 8	Grid 9
0.127	0.125	0.122		0.127	0.125	0.122

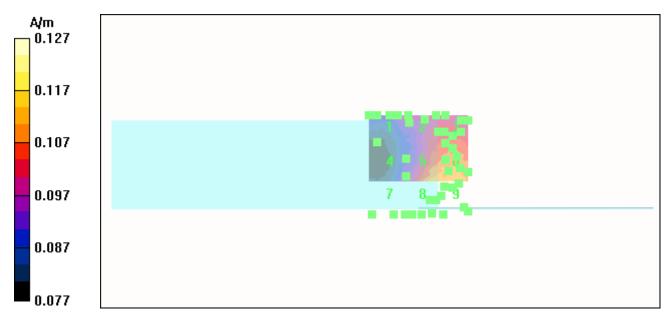



WR-905.001





40 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 9/1/2005 9:16:52 AM Test Laboratory: TCC Dallas

RM-59, CDMA800, Ch777, Whip Extend position, H field

Communication System: CDMA800; Frequency: 848.31 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0673 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.104 A/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

	`	0	<u>.</u>		`	0,
Grid 1	Grid 2	Grid 3		Grid 1	Grid 2	Grid 3
0.087	0.096	0.098		0.087	0.096	0.098
Grid 4	Grid 5	Grid 6		Grid 4	Grid 5	Grid 6
0.085	0.103	0.104		0.085	0.103	0.104
Grid 7	Grid 8	Grid 9		Grid 7	Grid 8	Grid 9
0.118	0.111	0.109		<mark>0.118</mark>	0.111	0.109

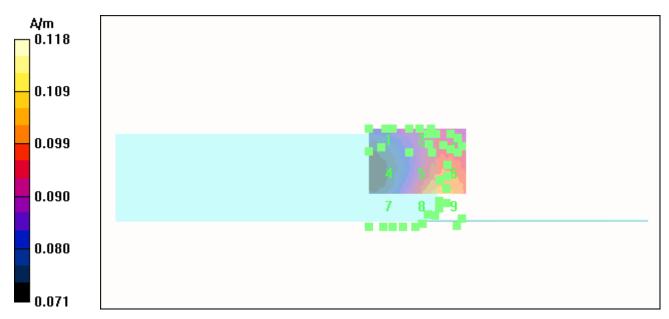



WR-905.001

Test & Certification Center (TCC) - Dallas

07 September 2005



41 (47)

Ver 1.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 8/31/2005 3:02:03 PM Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch25, Whip Extend position, E field

Communication System: CDMA1900; Frequency: 1851.25 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0184 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 27.1 V/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
27.4	24.5	19.1	27.4	24.5	19.1
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
26.2	25.8	22.1	26.2	25.8	22.1
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
28.2	27.1	22.9	28.2	27.1	22.9

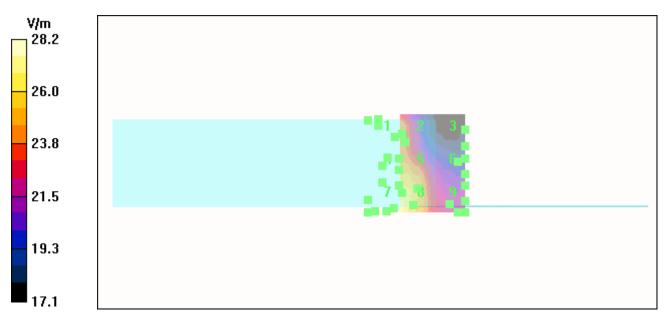



WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

42 (47)

07 September 2005

Date/Time: 8/31/2005 2:29:49 PM Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch600, Whip Extend position, E field

Communication System: CDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = 0.298 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 29.5 V/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
32.3	29.5	23.0	32.3	29.5	23.0
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
28.1	27.5	24.8	28.1	27.5	24.8
	27.5 Grid 8				24.8 Grid 9

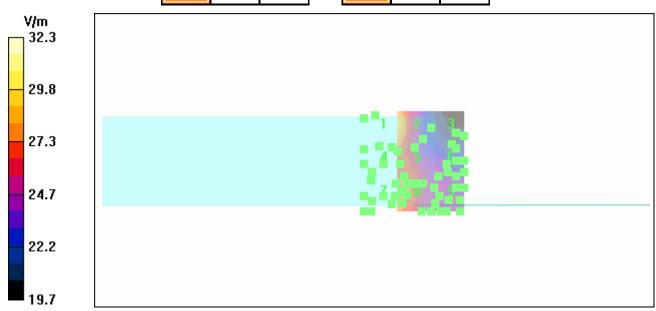



07 September 2005

WR-905.001



Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

43 (47)

Date/Time: 8/31/2005 3:24:56 PM Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch1175, Whip Extend position, E field

Communication System: CDMA1900; Frequency: 1908.75 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: ER3DV6 SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0551 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 30.5 V/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

			-			
Grid 1	Grid 2	Grid 3		Grid 1	Grid 2	Grid 3
31.0	25.3	23.4		31.0	25.3	23.4
Grid 4	Grid 5	Grid 6		Grid 4	Grid 5	Grid 6
28.2	26.9	24.3		28.2	26.9	24.3
Grid 7	Grid 8	Grid 9		Grid 7	Grid 8	Grid 9
32.0	30.5	25.4		32.0	30.5	25.4

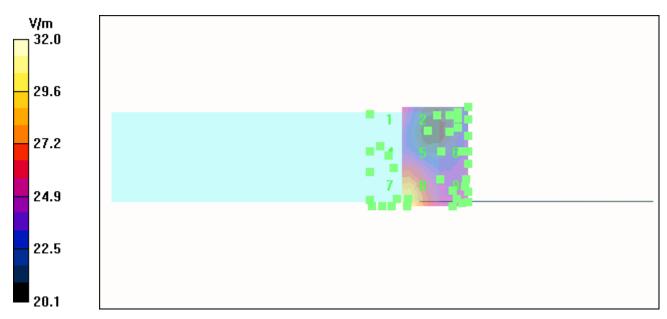



WR-905.001

Test & Certification Center (TCC) - Dallas

07 September 2005



Ver 1.0

44 (47)

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 9/1/2005 10:04:31 Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch25, Whip Extend position, H field

Communication System: CDMA1900; Frequency: 1851.25 MHz;Duty Cycle: 1:1 DASY4 Configuration:

- Probe: H3DV6 - SN6155; ; Calibrated: 2/16/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn389; Calibrated: 1/12/2005

- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section

- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146


Power Drift = 0.174 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.071 A/m

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 2 Grid 1 Grid 3 Grid 1 Grid 2 Grid 3 0.065 0.067 0.067 0.065 0.067 0.067 Grid 5 Grid 4 Grid 6 Grid 4 Grid 5 Grid 6 0.071 0.071 0.071 0.071 0.071 0.071 Grid 7 Grid 8 Grid 9 Grid 7 Grid 8 Grid 9 0.084 0.076 0.084 0.076 0.072 0.072

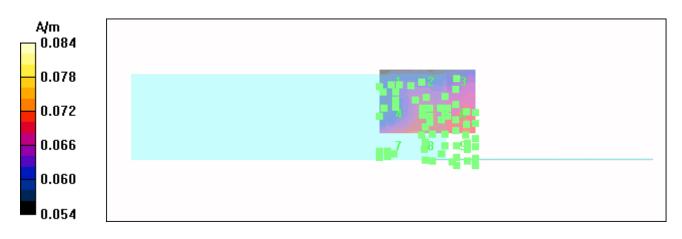



WR-905.001





45 (47)

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Ver 1.0

Date/Time: 9/1/2005 9:41:43 AM Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch600, Whip Extend position, H field

Communication System: CDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.214 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.081 A/mHearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

	`	9	<u> </u>		(5,
Grid 1	Grid 2	Grid 3		Grid 1	Grid 2	Grid 3
0.064	0.070	0.077		0.064	0.070	0.077
Grid 4	Grid 5	Grid 6		Grid 4	Grid 5	Grid 6
0.073	0.075	0.081		0.073	0.075	0.081
Grid 7	Grid 8	Grid 9		Grid 7	Grid 8	Grid 9
0.086	0.082	0.081		0.086	0.082	0.081

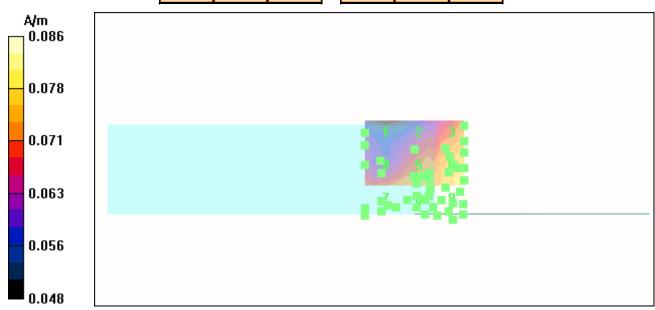



WR-905.001





46 (47)

Ver 1.0

Test & Certification Center (TCC) - Dallas

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 9/1/2005 10:24:57 AM Test Laboratory: TCC Dallas

RM-59, CDMA1900, Ch1175, Whip Extend position, H field

Communication System: CDMA1900; Frequency: 1908.75 MHz;Duty Cycle: 1:1 DASY4 Configuration:


- Probe: H3DV6 SN6155; ; Calibrated: 2/16/2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn389; Calibrated: 1/12/2005
- Phantom: SAM3 Cover FreeSpace Only; Phantom section: Table Section
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

Power Drift = -0.0628 dB

HAC Procedure/Hearing Aid Compatibility Test (251x251x1): Measurement grid: dx=2mm, dy=2mm Maximum value of Total field (slot averaged) = 0.080 A/m Hearing Aid Near-Field Category: M4 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

······································						
Grid 1	Grid 2	Grid 3		Grid 1	Grid 2	Grid 3
0.062	0.071	0.073		0.062	0.071	0.073
Grid 4	Grid 5	Grid 6		Grid 4	Grid 5	Grid 6
0.067	0.075	0.081		0.067	0.075	0.081
Grid 7	Grid 8	Grid 9		Grid 7	Grid 8	Grid 9
0.080	0.076	0.083		0.080	0.076	0.083

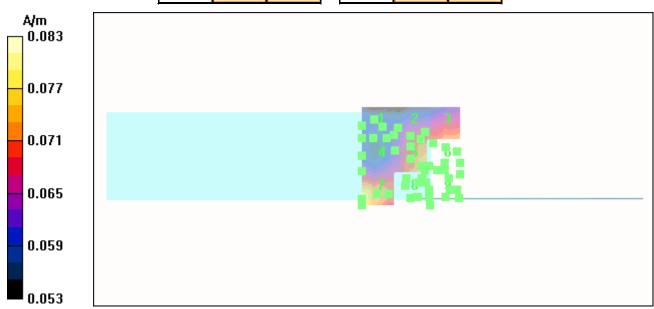



WR-905.001



Test & Certification Center (TCC) - Dallas

07 September 2005

Ver 1.0 Accredited Laboratory Certificate Number: 1819-01

APPENDIX C: PROBE CALIBRATION REPORTS AND DIPOLE CALIBRATION REPORTS

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Client Nokia TX	-	Certificate No:	ER3-2337_Jan05
CALIBRATION (CERTIFICAT		
Object	ER3DV6 - SN:2	337	
Calibration procedure(s)	QA CAL-02.v4 Calibration proc evaluations in ai	edure for E-field probes optimized for r	or close near field
Calibration date:	January 31, 200	5	
Condition of the calibrated item	In Tolerance		
		tional standards, which realize the physical units probability are given on the following pages and a	
All calibrations have been condu	cted in the closed laborate	bry facility: environment temperature (22 \pm 3)°C a	nd humidity < 70%.
Calibration Equipment used (M&	TE critical for calibration)		
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-May-04 (METAS, No. 251-00388)	May-05
Power sensor E4412A	MY41495277	5-May-04 (METAS, No. 251-00388)	May-05
Reference 3 dB Attenuator	SN: \$5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-04 (METAS, No. 251-00389)	May-05
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe ER3DV6	SN: 2328	6-Oct-04 (SPEAG, No. ER3-2328_Oct04)	Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Jan05)	Jan-06
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct 05
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05
	Nama		Dispeture
Calibrated by:	Name Katja Pokovic	Function Technical Manager	Signature
		r Animiral Manafai	plai = lat-
Approved by:	Niels Kuster	Quality Manager	1.165
			Issued: February 19, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst S

- Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S **Swiss Calibration Service**

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx,y,z	sensitivity in free space
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization 9	arsigma rotation around an axis that is in the plane normal to probe axis (at
	measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1309-1996, " IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization $\vartheta = 0$ for XY sensors and $\vartheta = 90$ for Z sensor (f \leq 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x, y, z = NORMx, y, z * frequency response (see Frequency Response Chart).
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of . power sweep (no uncertainty required). DCP does not depend on frequency.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized • using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center • from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Probe ER3DV6

SN:2337

Manufactured: Calibrated: September 9, 2003 January 31, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)


ER3DV6 SN:2337

DASY - Parameters of Probe: ER3DV6 SN:2337

Sensitivity in	Free Space [µV	/(V/m) ²]	Diod	e Compression	A
Norm	X 1.51 ± 1	0.1 % (k=2)	DCP	X 95 mV	
Norm	Y 1.43 ± 1	0.1 % (k=2)	DCP	Y 95 mV	
Norm	Z 1.58 ± 1	0.1 % (k=2)	DCP	Z 97 mV	
Frequency C	orrection				
х		0.0			
Y		0.0			
Z		0.0			
Sensor Offse	et (Pr	obe Tip to Senso	r Center)		
х		2.5 mm			
Y		2.5 mm			
Z		2.5 mm			
Connector A	ngle	-25 °			

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


^A numerical linearization parameter: uncertainty not required

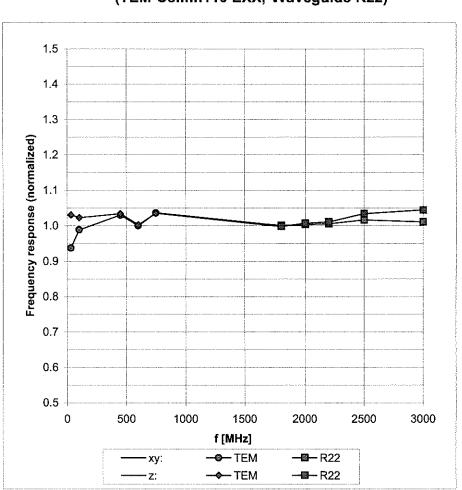

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide R22)


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

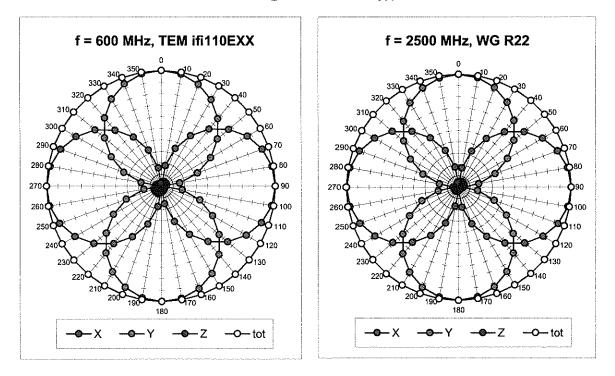

Receiving Pattern (ϕ **),** ϑ = 0°


Receiving Pattern (ϕ **),** ϑ = 90°

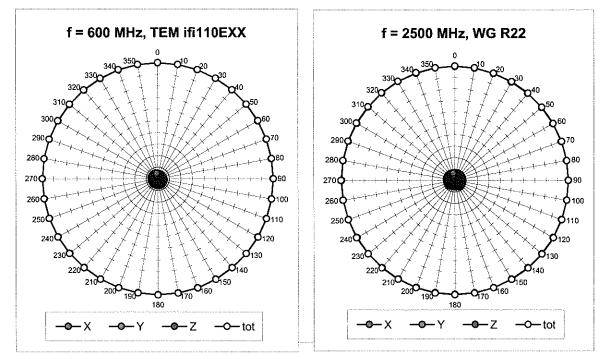

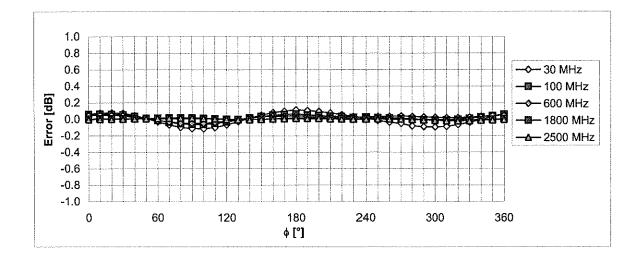


Receiving Pattern (ϕ **),** ϑ = 0°

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

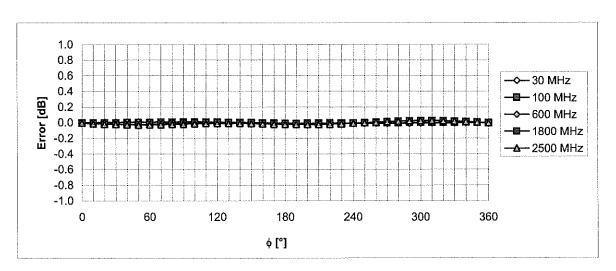


Receiving Pattern (ϕ **),** ϑ = 90°


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

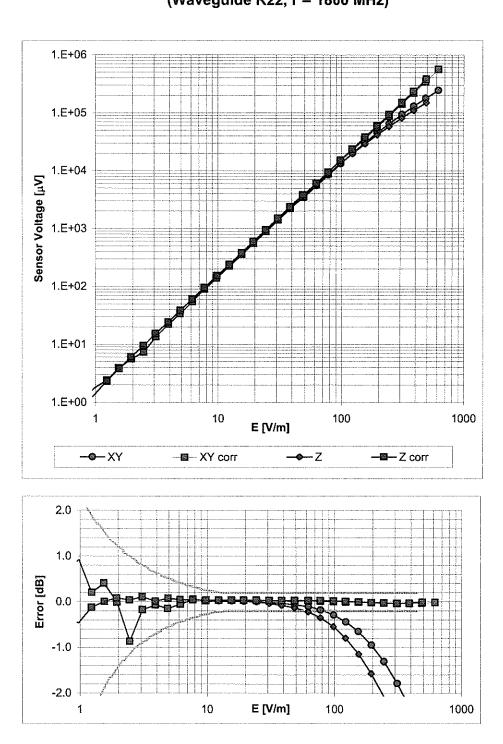

Dynamic Range f(E-field) (Waveguide R22, f = 1800 MHz)

Uncertainty of Linearity Assessment: ± 0.6% (k=2)



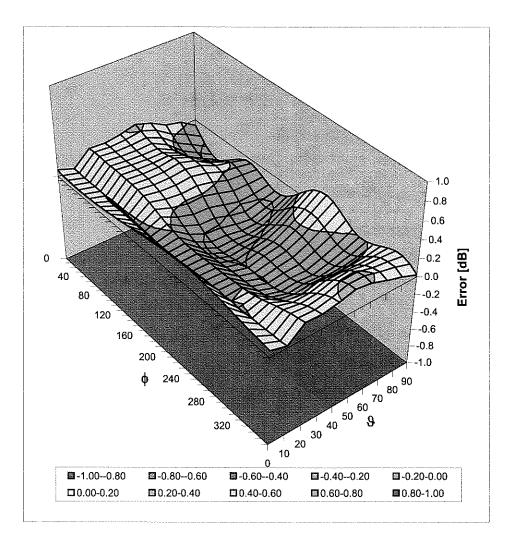

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland

aWIS.

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Continuo No. H3-6155 Fab05

Accreditation No.: SCS 108

S

С

S

Client Nokia TX		Certificate	e No: H3-6155_Feb05
CALIBRATION	BERTIFICAT	E	
Object	H3DV6 - SN:61	55	
Calibration procedure(s)	QA CAL-03.v4 Calibration proc evaluations in ai	edure for H-field probes optimiz r	red for close near field
Calibration date:	February 16, 20	05	
Condition of the calibrated item	In Tolerance		
		tional standards, which realize the physica probability are given on the following pages	
All calibrations have been conduc	cted in the closed laborate	ory facility: environment temperature (22 \pm	3)°C and humidity < 70%.
Calibration Equipment used (M&	TE critical for calibration)		
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.	.) Scheduled Calibration
Power meter E4419B	GB41293874	5-May-04 (METAS, No. 251-00388)	May-05
Power sensor E4412A	MY41495277	5-May-04 (METAS, No. 251-00388)	May-05
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-04 (METAS, No. 251-00389)	May-05
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe H3DV6	SN: 6182	6-Oct-04 (SPEAG, No. H3-6182_Oct04	4) Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Ja	an05) Jan-06
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check O	ct-03) In house check: Oct 05
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check De	c-03) In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check No	ov-04) In house check: Nov 05
		Function	
Calibrated by:	Katja Pokovic	Technical Manager	Apri- Unt
Approved by:	Niels Kuster	Quality Manager	X. Lots
This calibration certificate shall n		n full without written approval of the labora	Issued: February 19, 2005

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S

Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
- Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx,y,z	sensitivity in free space
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization 9	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1309-1996, " IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

Methods Applied and Interpretation of Parameters:

- X,Y,Z_a0a1a2: Assessed for E-field polarization θ = 90 for XY sensors and θ = 0 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- X,Y,Z(f)_a0a1a2= X,Y,Z_a0a1a2* frequency_response (see Frequency Response Chart).
- *DCPx,y,z:* DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *X_a0a1a2* (no uncertainty required).

Probe H3DV6

SN:6155

Manufactured: Calibrated: June 22, 2004 February 16, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)


H3DV6 SN:6155

DASY - Parameters of Probe: H3DV6 SN:6155

Sensitivity in Fr	ee Space	[A/m / √(µV))]
	a0	a1 a	a2
Х	2.719E-03	-7.681E-5	3.643E-5 ± 5.1 % (k=2)
Y	2.743E-03	1.819E-5	-1.877E-5 ± 5.1 % (k=2)
Z	2.974E-03	-4.287E-5	-1.156E-5 ± 5.1 % (k=2)
Diode Compres	sion ¹		
DCP X 8	6 mV		
DCP Y 8	6 mV		
DCP Z 8	5 mV		
Sensor Offset		(Probe Tip to	Sensor Center)
х		3.0	mm
Y		3.0	mm
Z		3.0	mm
Connector Ang	le	319 '	D

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


¹ numerical linearization parameter: uncertainty not required

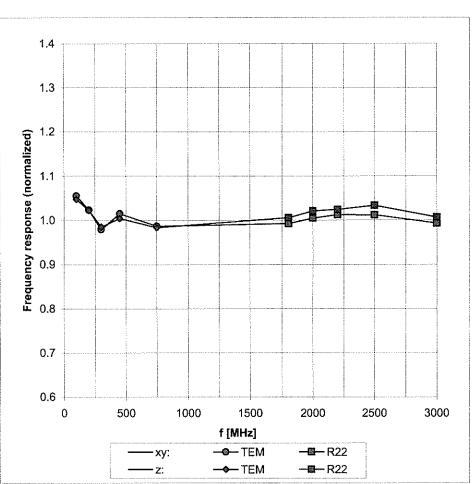

Frequency Response of H-Field


(TEM-Cell:ifi110, Waveguide R22)


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

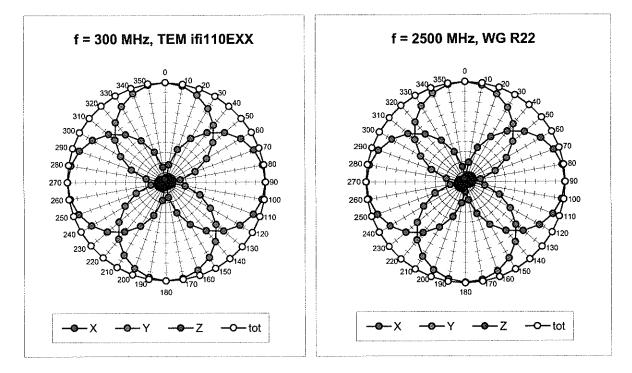

Receiving Pattern (ϕ), ϑ = 90°


Receiving Pattern (ϕ **),** ϑ = 0°

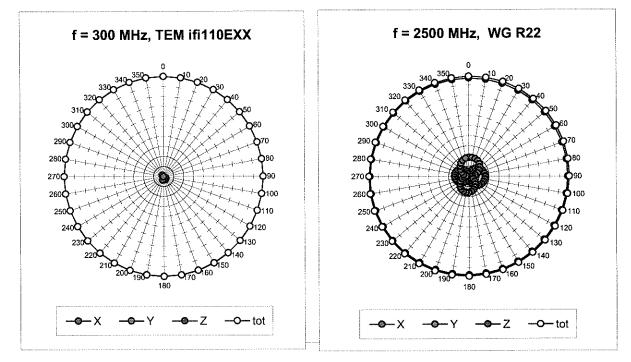

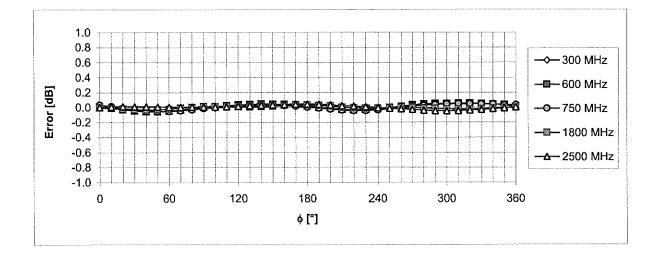


Receiving Pattern (ϕ), ϑ = 90°

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

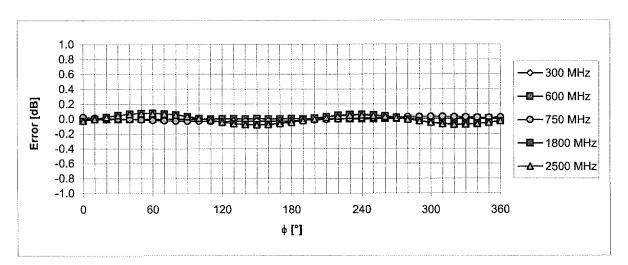

Receiving Pattern (ϕ **),** ϑ = 0°

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

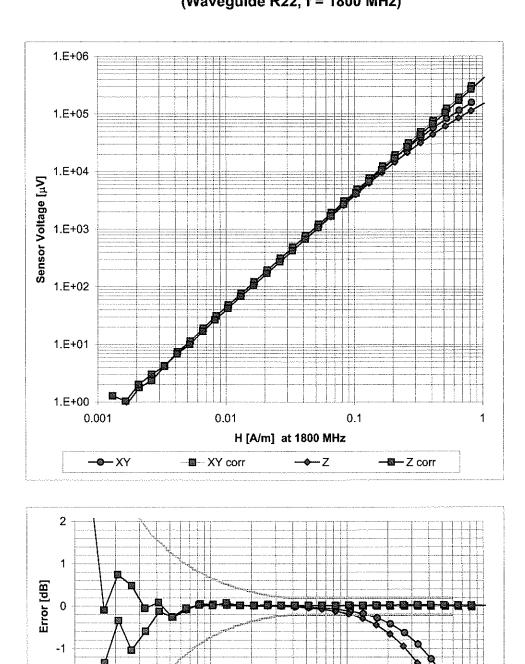

Dynamic Range f(H-field) (Waveguide R22, f = 1800 MHz)

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

H [A/m] at 1800 MHz

0.1

1

-2 0.001

0.01

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Nokia TX

Certificate No: CD835V3-1032_Apr05

Object CD835V3 - SN: 1032 Calibration procedure(s) QA CAL-20.V3 Calibration procedure for dipoles in air Calibration date: April 27, 2005 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). Al calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). Al calibration stave been conclusted at an environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Prower meter EPM4420A CB3740704 12-Oct-04 (METAS, No. 251-00412) Oct-05 20 dB Attenuator SN: 5068 (20g) 10-Aug-04 (METAS, No. 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) in house check: Oct-05 Power sensor HP 8481A MY41092315 10-Aug-03 (SPEAG, in house check Aug-04) in house check: Oct-05 <th>CALIBRATION C</th> <th>ERTIFICAT</th> <th>E</th> <th></th>	CALIBRATION C	ERTIFICAT	E	
Calibration procedure for dipoles in air Calibration date: April 27, 2005 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). All calibrations have been conducted at an environment temperature (22 ± 3)°C and humidity < 70%.	Object	CD835V3 - SN:	1032	
Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). All calibrations have been conducted at an environment temperature (22 ± 3)*C and humidity < 70%.	Calibration procedure(s)		edure for dipoles in air	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). All calibrations have been conducted at an environment temperature (22 ± 3)*C and humidity < 70%.	Calibration date:	April 27, 2005		
All calibrations have been conducted at an environment temperature (22 ± 3)*C and humidity < 70%.	Condition of the calibrated item	In Tolerance		
Power meter EPM-442A GB37480704 12-Oct-04 (METAS, No. 251-00412) Oct-05 Power sensor HP 8481A US37292783 12-Oct-04 (METAS, No. 251-00412) Oct-05 20 dB Attenuator SN: 5086 (20g) 10-Aug-04 (METAS, No. 251-00402) Aug-05 10 dB Attenuator SN: 5047.2 (10r) 10-Aug-04 (METAS, No. 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power meter EPM-4419B GB43310788 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Nu-04) In house check: Nov-05 RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Inn-06 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 Probe H3DV6 SN: 8065 10-Dec-04 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06 Calibrated by: Name Function Si	All calibrations have been conduc	cted at an environment te	emperature (22 ± 3)°C and humidity < 70%.	f measurements (SI).
Power sensor HP 8481A US37292783 12-Oct-04 (METAS, No. 251-00412) Oct-05 20 dB Attenuator SN: 5086 (20g) 10-Aug-04 (METAS, No 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092315 10-Aug-03 (SPEAG, in house check Nov-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 J039.2000.06 26-Jul-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 Calibrated by: Name Function Signature Calibrated by: Name Function Signature Approved by: Fin Bornholt Technical Director Technical Director Susced: June 13, 2005 In 2010 Insue Insue	Primary Standards	1D #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power sensor HP 8481A US37292783 12-Oct-04 (METAS, No. 251-00412) Oct-05 20 dB Attenuator SN: 5086 (20g) 10-Aug-04 (METAS, No. 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power meter EPM-4419B GB43310788 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 D39.2000.06 26-Jul-04 (SPEAG, No. DAE4-901_un04) Calibration, Jun-05 Calibration SN: 2036 20-Jan-05 (SPEAG, No. H3-6065-Dec04) Calibration, Jan-06 Calibrated by: Name Function Signature Approved by: Fin Bomholt Technical Director Technical Director Susced: June 13, 2005 Susced: June 13, 2005 Susced: June 13, 2005				Oct-05
20 dB Attenuator SN: 5086 (20g) 10-Aug-04 (METAS, No 251-00402) Aug-05 10 dB Attenuator SN: 5047.2 (10r) 10-Aug-04 (METAS, No 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power meter EPM-4419B GB43310788 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 CAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jan-06 Probe ER3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Jan-06 Calibrated by: Name Function Signature Calibrated by: Fin Bomholt Technical Director FM2MULL Approved by: Fin Bomholt Technical Director FM2MULL	Power sensor HP 8481A		•	
N0 dB Attenuator SN: 5047.2 (10r) 10-Aug-04 (METAS, No 251-00402) Aug-05 Secondary Standards ID # Check Date (in house) Scheduled Check Power meter EPM-4419B GB43310788 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Nov-05 Reperator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Nov-05 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 Calebrated by: SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Calibrated by: Fin Bomholt Technical Director Technical Director Approved by: Fin Bomholt Technical Director Tech	20 dB Attenuator	SN: 5086 (20a)		Aua-05
Power meter EPM-4419B GB43310788 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 OAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jan-06 OAE4 SN: 901 29-Jun-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06 Probe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Calibrated by: Nike Meill Technical Director Technical Director Approved by: Fin Bomholt Technical Director Technical Director	0 dB Attenuator	, ,		-
Power sensor HP 8481A MY41092312 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Jan-04) In house check: Oct-05 RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Jan-06 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) In house check: Jan-06 Probe ER3DV6 SN: 2336 20-Jan-05 (SPEAG, No. H3-6065-Dec04) Calibration, Jan-06 Probe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Approved by: Fin Bomholt Technical Director FLOUID Approved by: Fin Bomholt Technical Director FLOUID	Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A MY41093315 10-Aug-03 (SPEAG, in house check Jan-04) In house check: Oct-05 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 D39.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Nov-05 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) In house check: Jan-06 Date SN: 2036 20-Jan-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06 Drobe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Approved by: Fin Bomholt Technical Director Fundult Approved by: Fin Bomholt Technical Director Fundult	Power meter EPM-4419B	GB43310788	10-Aug-03 (SPEAG, in house check Jan-04)	In house check: Oct-05
Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Jan-06 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) In house check: Jan-06 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 Drobe ER3DV6 SN: 2336 20-Jan-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06 Drobe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Mike Meili Laboratory Technician Technical Director The Midu Approved by: Fin Bomholt Technical Director The Midu Issued: June 13, 2005 Issued: June 13, 2005 Issued: June 13, 2005	Power sensor HP 8481A	MY41092312	10-Aug-03 (SPEAG, in house check Jan-04)	In house check: Oct-05
Name Function Signature Name Function Signature Mike Meili Laboratory Technician Signature Supproved by: Fin Bomholt Technical Director Function Sup	ower sensor HP 8481A	MY41093315	10-Aug-03 (SPEAG, in house check Jan-04)	In house check: Oct-05
RF generator R&S SMT06 1039.2000.06 26-Jul-04 (SPEAG, in house check Jul-04) In house check: Jan-06 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) In house check: Jan-06 Drobe ER3DV6 SN: 2336 20-Jan-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jun-05 Drobe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Jun-05 Calibrated by: Name Function Signature Mike Meili Laboratory Technician Signature Approved by: Fin Bomholt Technical Director Fundult Issued: June 13, 2005 Issued: June 13, 2005 Issued: June 13, 2005	letwork Analyzer HP 8753E	US37390585		In house check: Nov-05
DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05 Drobe ER3DV6 SN: 2336 20-Jan-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06 Drobe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Mike Melli Laboratory Technician Thefici Approved by: Fin Bomholt Technical Director Function Issued: June 13, 2005 Sued: June 13, 2005	RF generator R&S SMT06	1039.2000.06	26-Jul-04 (SPEAG, in house check Jul-04)	In house check: Jan-06
Probe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Mike Meili Laboratory Technician M.T.E.L. Approved by: Fin Bomholt Technical Director F.M.M.M.L. Issued: June 13, 2005 June 13, 2005 June 13, 2005	DAE4	SN: 901		Calibration, Jun-05
Probe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05 Calibrated by: Name Function Signature Mike Meili Laboratory Technician M.T.B.J.J. Approved by: Fin Bomholt Technical Director F.M.M.M. Issued: June 13, 2005 June 13, 2005 June 13, 2005	Probe ER3DV6	SN: 2336	20-Jan-05 (SPEAG, No. ER3-2336 Jan05)	Calibration, Jan-06
Calibrated by: Mike Meili Laboratory Technician D. Deili Approved by: Fin Bomholt Technical Director F. Multiple Issued: June 13, 2005 Issued: June 13, 2005	Probe H3DV6	SN: 6065		Calibration, Dec-05
Approved by: Fin Bomholt Technical Director F. Smillit Issued: June 13, 2005		Name	Function	Signature
Issued: June 13, 2005	Calibrated by:	Mike Meili	Laboratory Technician	n. Teiji
	Approved by:	Fin Bomholt	Technical Director	Bmhilt
				Issued: June 13, 2005
This calibration certificate is issued as an intermediate solution until the specific calibration procedure is accepted in the frame of the accreditation of the Calibration Laboratory of Schmid & Partner Engineering AG (based on ISO/IEC 17025 International Standard)			, , , , , , , , , , , , , , , , , , ,	•

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

References

 ANSI-PC63.19-2001 (Draft 3.x, 2005)
 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with standard [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the the top edge of the dipole arms.
- *Measurement Conditions:* Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections.
 It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY4 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- *E- field distribution:* E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- *H-field distribution:* H-field is measured with an isotropic H-field probe with 100mW forward power to the antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the feed point.

1 Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.5 B19
DASY PP Version	SEMCAD	V1.8 B149
Phantom	HAC Test Arch SD HAC P01 BA	
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 180 mm
Frequency	835 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

2 Maximum Field values

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW forward power	0.451 A/m
Uncertainty for H-field measurement: 8.2% (k=2)	Aussen and a second	

E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW forward power	163.8 V/m
Maximum measured above low end	100 mW forward power	160.4 V/m
Averaged maximum above arm	100 mW forward power	162.1 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

3 Appendix

3.1 Antenna Parameters

Frequency	Return Loss	Impedance
800 MHz	17.1 dB	(40.6. – j8.5) Ohm
835 MHz	27.5 dB	(51.1 + j4.1) Ohm
900 MHz	17.2 dB	(49.5 - j13.9) Ohm
950 MHz	18.7 dB	(55.2 + j11.1) Ohm
960 MHz	14.0 dB	(67.6 + j15.6) Ohm

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.


The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

3.3 Measurement Sheets

3.3.1 Return Loss and Smith Chart

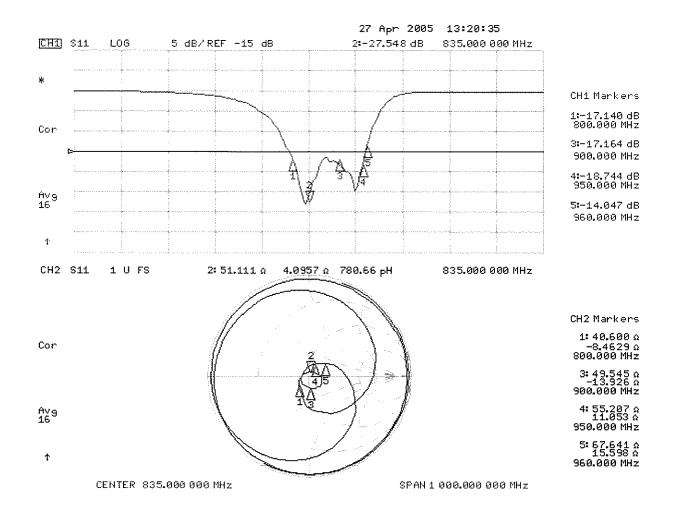

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1032

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$; $\rho = 1$ kg/m³ Phantom section: H Dipole Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: H3DV6 SN6065; ; Calibrated: 10.12.2004 ۰
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn901; Calibrated: 29.06.2004 ٠
- Phantom: HAC Phantom; Type: SD HAC P01 BA; •
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 149


H Scan 10mm above CD 835 MHz/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mmMaximum value of Total field (slot averaged) = 0.451 A/mReference Value = 0.473 A/m; Power Drift = -0.01 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 1	Grid 2	Grid 3	Grid 1	Grid 2	Grid 3
0.365	0.397	0.380	0.365	0.397	0.380
Grid 4	Grid 5	Grid 6	Grid 4	Grid 5	Grid 6
0.415	0.451	0.433	0.415	0.451	0.433
	Grid 8		Grid 7	Grid 8	Grid 9
0.363	0.395	0.380	0.363	0.395	0.380

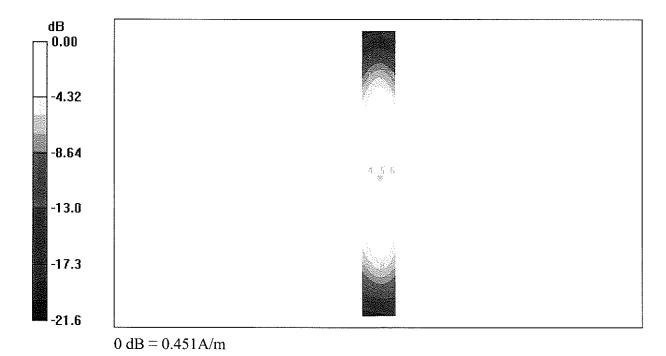

Contificate No. CD0251/2 1022

3.3.3 DASY4 E-Field result

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1032

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$; $\rho = 1000$ kg/m³ Phantom section: E Dipole Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ER3DV6 SN2336; ConvF(1, 1, 1); Calibrated: 20.01.2005
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn901; Calibrated: 29.06.2004
- Phantom: HAC Phantom; Type: SD HAC P01 BA;
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 149

E Scan 10mm above CD 835 MHz/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm


Maximum value of Total field (slot averaged) = 163.8 V/m

Reference Value = 102.7 V/m; Power Drift = -0.017 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

		, onugod)	 	. (0101 41	eragea)
Grid I	Grid 2	Grid 3	Grid 1		
156.6	160.4	153.8	156.6	160.4	153.8
	Grid 5		Grid 4		
85.9	88.0	84.1	85.9	88.0	84.1
Grid 7	Grid 8	Grid 9	Grid 7	Grid 8	Grid 9
157.9	163.8	159.6	157.9	163.8	159.6

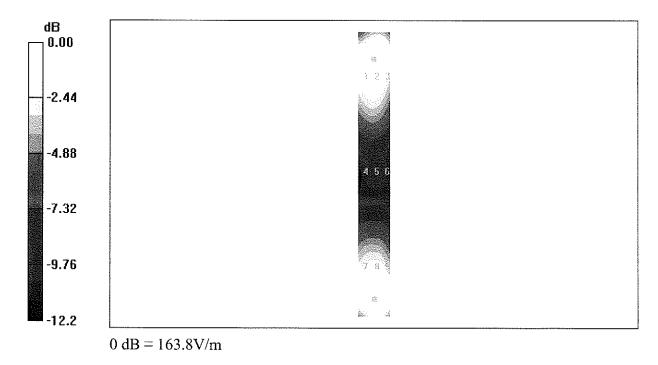

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Nokia TX

Certificate No: CD1880V3-1025_Jun05

	ERTIFICAT	на у на село село село су макета на село на село на село на село село село село село село село на село село на На село село село село село село село село	
Dbject	CD1880V3 - SN	: 1025	
Calibration procedure(s)	QA CAL-20.v3 Calibration proc	edure for dipoles in air	
alibration date:	June 2, 2005		
Condition of the calibrated item	In Tolerance		
	ted at an environment te	tional standards, which realize the physical units of emperature (22 \pm 3)°C and humidity < 70%.	measurements (SI).
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
ower meter EPM-442A	GB37480704	12-Oct-04 (METAS, No. 251-00412)	Oct-05
ower sensor HP 8481A	US37292783	12-Oct-04 (METAS, No. 251-00412)	Oct-05
) dB Attenuator	SN: 5086 (20g)	10-Aug-04 (METAS, No 251-00402)	Aug-05
0 dB Attenuator	SN: 5047.2 (10r)	10-Aug-04 (METAS, No 251-00402)	Aug-05
econdary Standards	ID #	Check Date (in house)	Scheduled Check
etwork Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov-05
F generator R&S SML-03	100698	27-Mar-02 (SPEAG, in house check Dec-03)	In house check: Dec-05
r yeneralur nað ðivil-uð	SN: 901		Calibration, Jun-05
•	314. 901	29-Jun-04 (SPEAG, No. DAE4-901_Jun04)	· · · · · · · · · · · · · · · · · · ·
AE4	SN: 2336	29-Jun-04 (SPEAG, No. DAE4-901_Jun04) 20-Jan-05 (SPEAG, No. ER3-2336_Jan05)	Calibration, Jan-06
Probe H3DV6			,
DAE4 Probe ER3DV6	SN: 2336	20-Jan-05 (SPEAG, No. ER3-2336_Jan05)	Calibration, Jan-06
AE4 robe ER3DV6 robe H3DV6	SN: 2336 SN: 6065	20-Jan-05 (SPEAG, No. ER3-2336_Jan05) 10-Dec-04 (SPEAG, No. H3-6065-Dec04)	Calibration, Jan-06 Calibration, Dec-05
DAE4 Probe ER3DV6	SN: 2336 SN: 6065 Name	20-Jan-05 (SPEAG, No. ER3-2336_Jan05) 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Function Laboratory Technician	Calibration, Jan-06 Calibration, Dec-05 Signature

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

References

 [1] ANSI-PC63.19-2001 (Draft 3.x, 2005)
 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with standard [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections.
 It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY4 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- *E- field distribution:* E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- *H-field distribution:* H-field is measured with an isotropic H-field probe with 100mW forward power to the antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the feed point.

1 Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.5 B31
DASY PP Version	SEMCAD	V1.8 B149
Phantom	HAC Test Arch	SD HAC P01 BA, #1002
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 90 mm
Frequency	1880 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

2 Maximum Field values

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW forward power	0.452 A/m
Less de la field mener print 9.00/ /k=2)		

Uncertainty for H-field measurement: 8.2% (k=2)

E-field 10 mm above dipole surface	condition	interpolated maximum	
Maximum measured above high end	100 mW forward power	139.4 V/m	
Maximum measured above low end	100 mW forward power	135.8 V/m	
Averaged maximum above arm	100 mW forward power	137.6 V/m	

Uncertainty for E-field measurement: 12.8% (k=2)

3 Appendix

3.1 Antenna Parameters

Frequency	Return Loss	Impedance
1710 MHz	19.9 dB	(61.2 – j0.7) Ohm
1880 MHz	20.9 dB	(58.6 – j4.7) Ohm
1900 MHz	21.7 dB	(55.5 – j6.7) Ohm
1950 MHz	30.4 dB	(49.0 – j2.8) Ohm
2000 MHz	21.0 dB	(54.0 + j8.4) Ohm

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.


The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

3.3 Measurement Sheets

3.3.1 Return Loss and Smith Chart

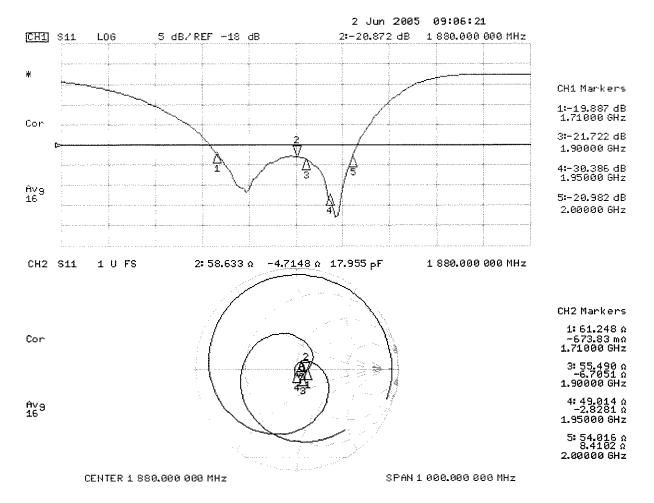

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1025

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³ Phantom section: H Dipole Section

DASY4 Configuration:

- Probe: H3DV6 SN6065; Calibrated: 12/10/2004
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn901; Calibrated: 6/29/2004
- Phantom: HAC Test Arch; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.5 Build 31; Postprocessing SW: SEMCAD, V1.8 Build 149

H Scan 10mm above CD1880V3/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm


Maximum value of Total field (slot averaged) = 0.452 A/m

Reference Value = 0.478 A/m; Power Drift = -0.034 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 2 0.425	t	 Grid 2 0.425	
 Grid 5 0.452		Grid 5 0.452	
Grid 8 0.401		Grid 8 0.401	

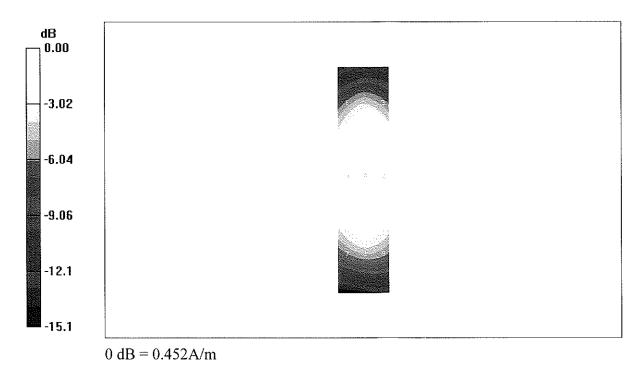

3.3.3 DASY4 E-Field result

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1025

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$; $\rho = 1000$ kg/m³ Phantom section: E Dipole Section

DASY4 Configuration:

- Probe: ER3DV6 SN2336; ConvF(1, 1, 1); Calibrated: 1/20/2005 •
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn901; Calibrated: 6/29/2004
- Phantom: HAC Test Arch; Type: SD HAC P01 BA; Serial: 1002
- Measurement SW: DASY4, V4.5 Build 31; Postprocessing SW: SEMCAD, V1.8 Build 149

E Scan 10mm above CD1880V3/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm


Maximum value of Total field (slot averaged) = 139.4 V/m

Reference Value = 157.2 V/m; Power Drift = 0.013 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

	Grid 2 135.8		Grid 1 131.9		
Grid 4 90.0			Grid 4 90.0	Grid 5 91.6	
	Grid 8 1 39.4		Grid 7 131.8		

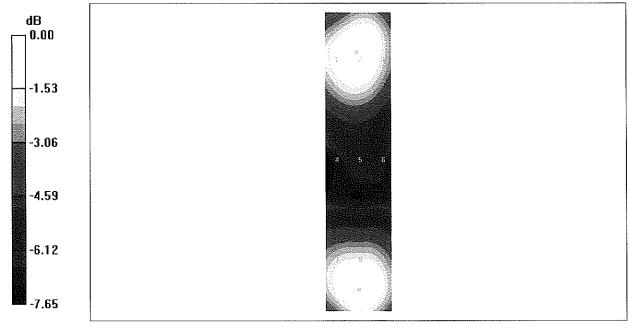

0 dB = 139.4 V/m