


 Medkonsult Medical Technology	Device marking FU8002-915	Valid from: 20.11.2023
		Verze 02/2023


1 DEVICE MARKING

1.1 List of a labels

1. Product and FCC štítek
2. Serial number

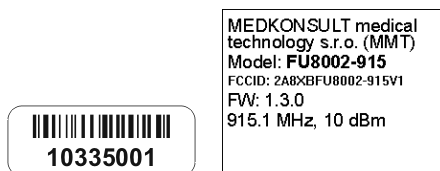

1.2 Device marking positioning

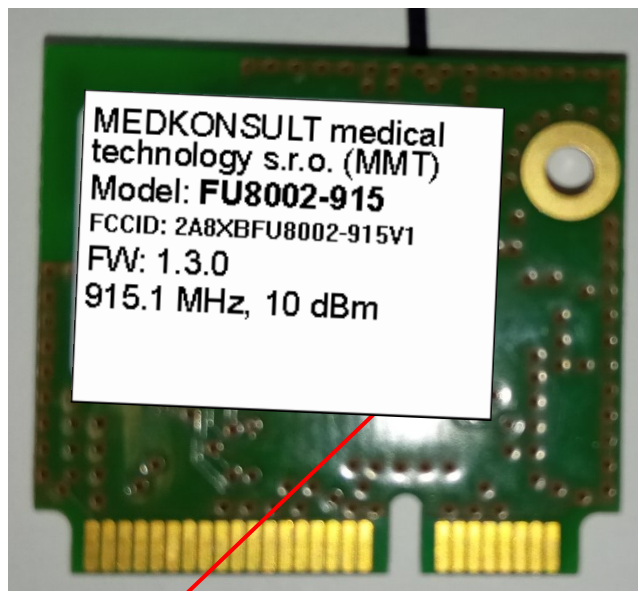

1



2