

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

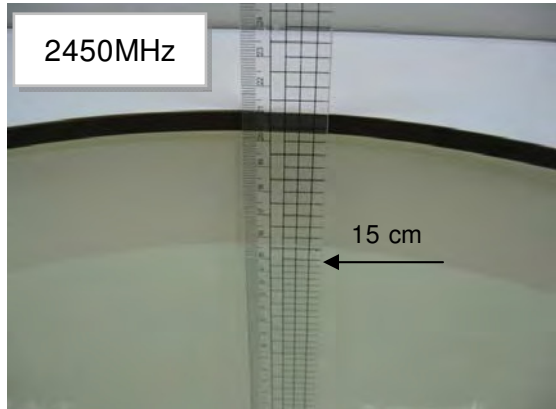


Fig.2.1

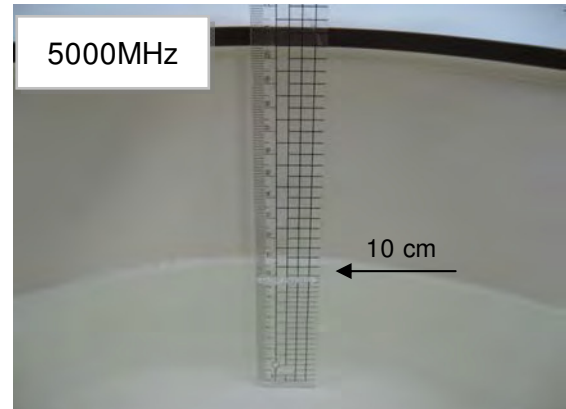


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm



Fig.3 EUT Top side to flat phantom

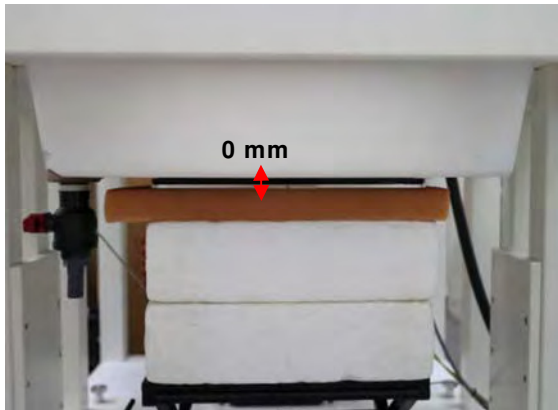
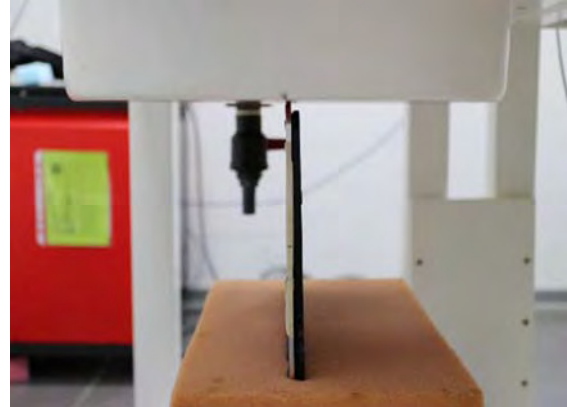


Fig.4 EUT Back side to flat phantom


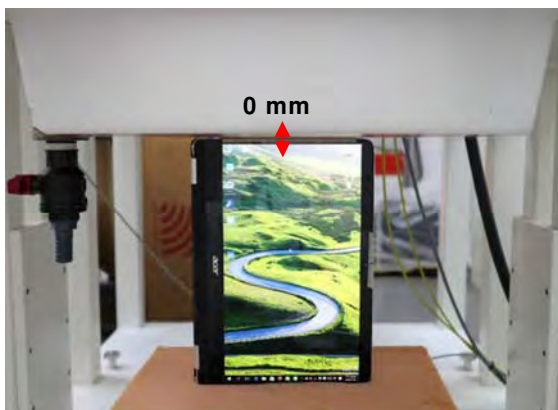


Fig.5 EUT Left side to flat phantom

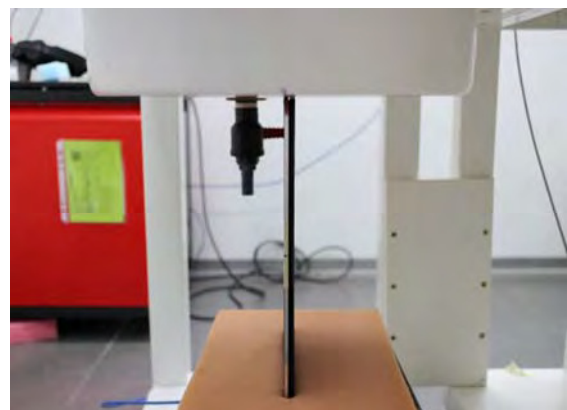

12. Photographs of the EUT



Fig.6 Front view of EUT



Fig.7 Laptop mode

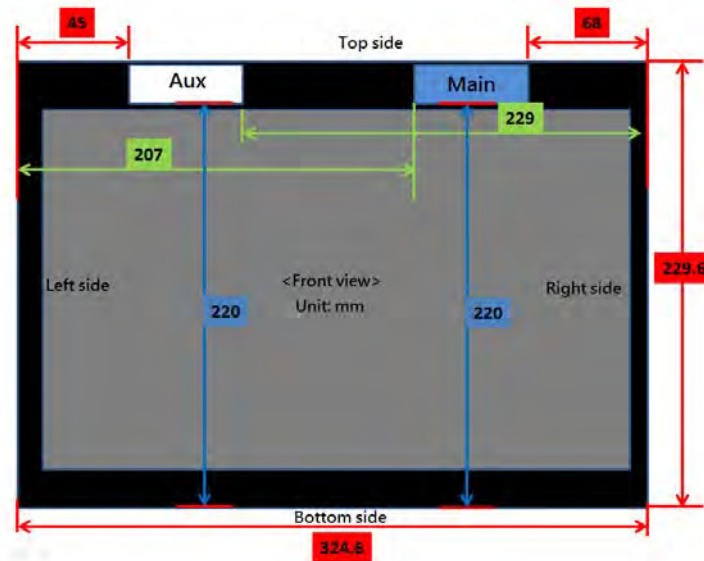


Fig.8 Antenna location of tablet mode



Fig.9 Edge view of tablet mode

- End of Report -