



Appendix D

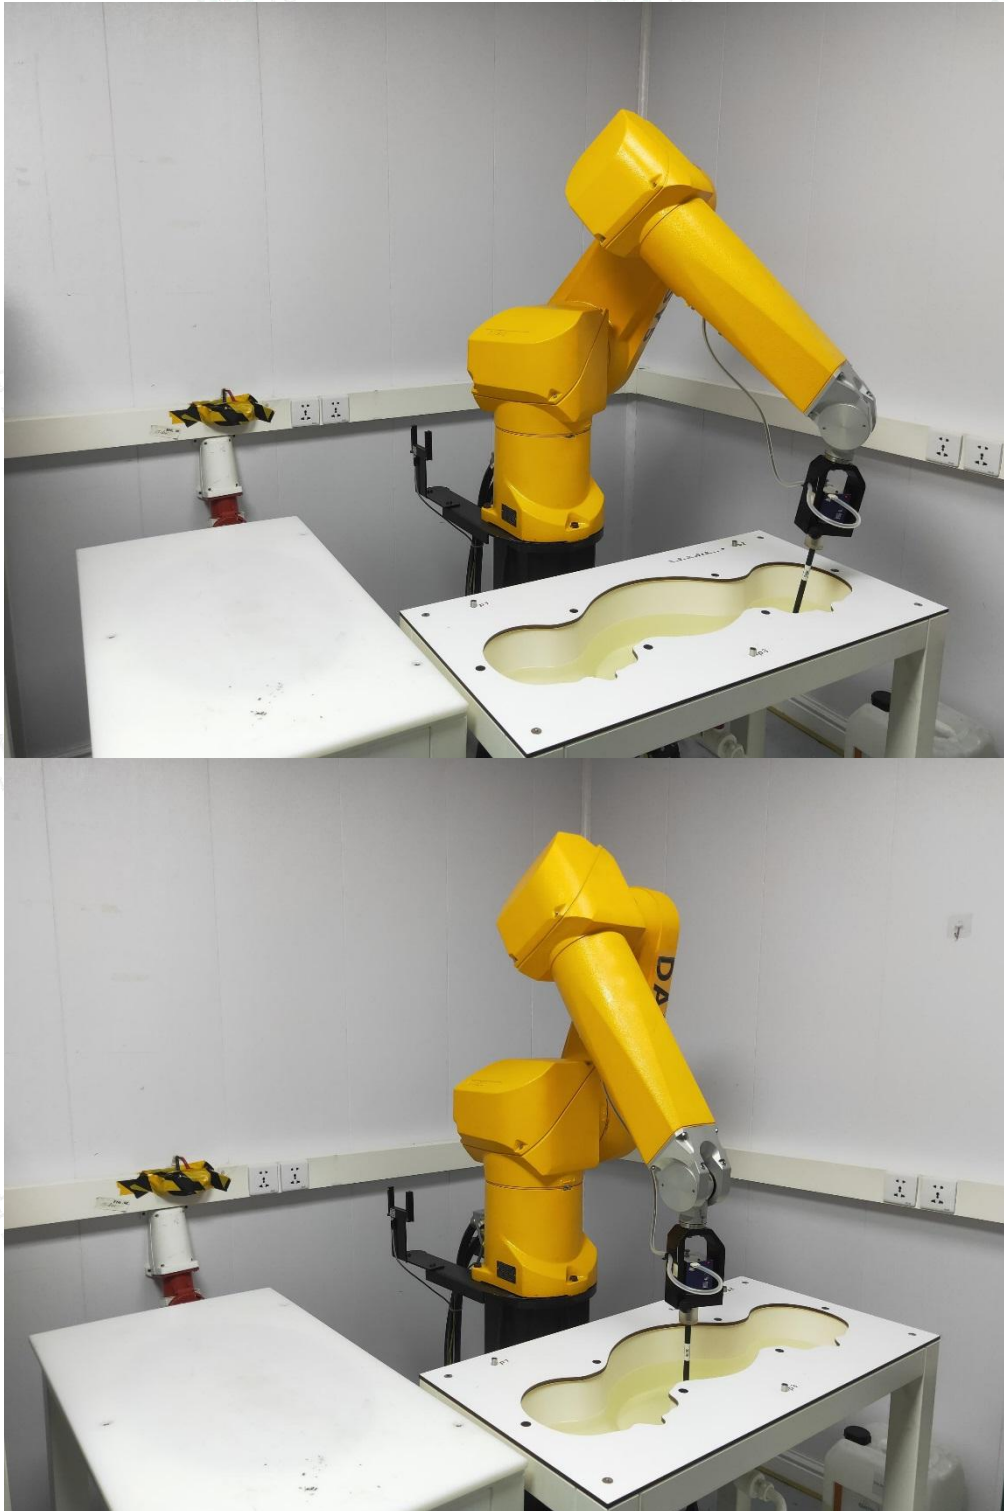
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details



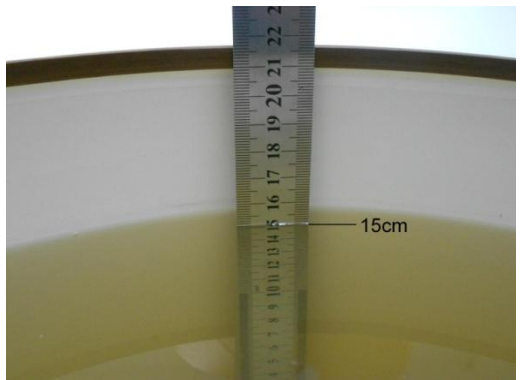
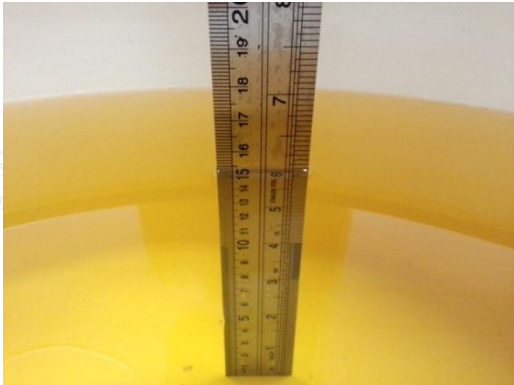
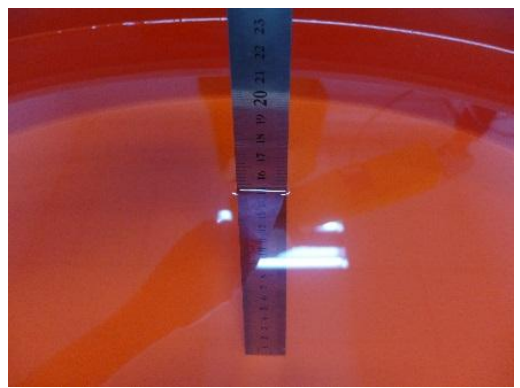


1. SAR measurement System





2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 5000
	





3. Photographs of EUT test position

Photo 7: Front side 0mm



Photo 8: Back side 0mm



Photo 9: Left side 0mm



Photo 10: Right side 0mm



Photo 11: Top side 0mm



Photo 12: Bottom side 0mm





4. EUT Constructional Details

