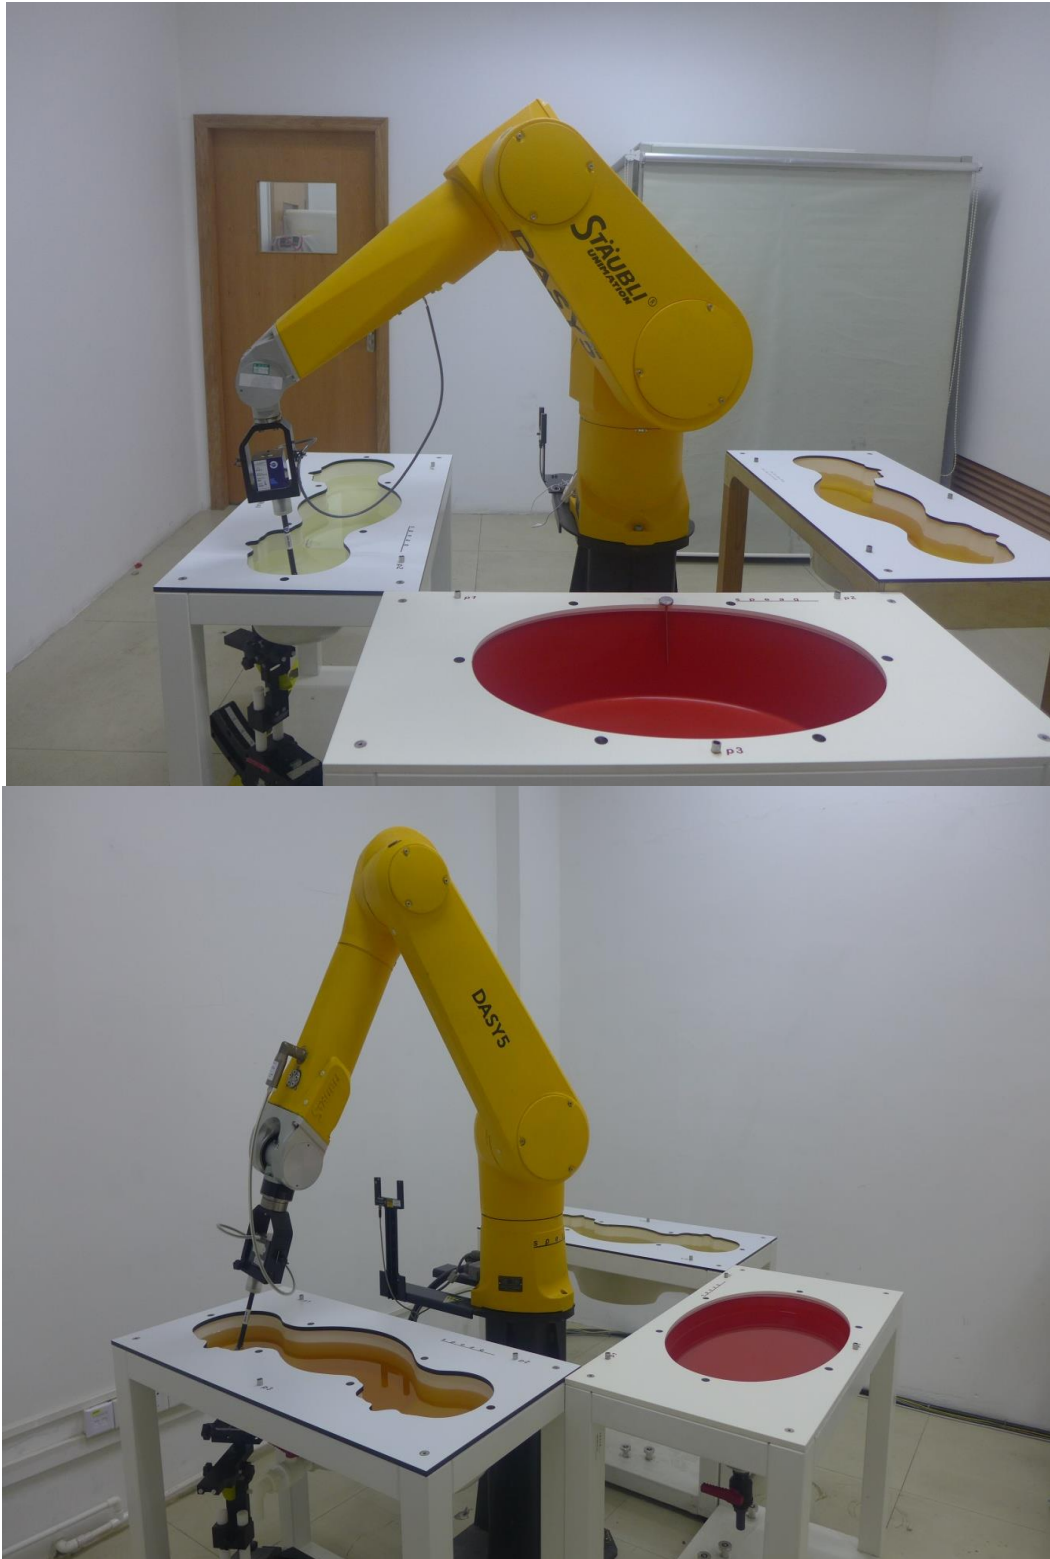


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

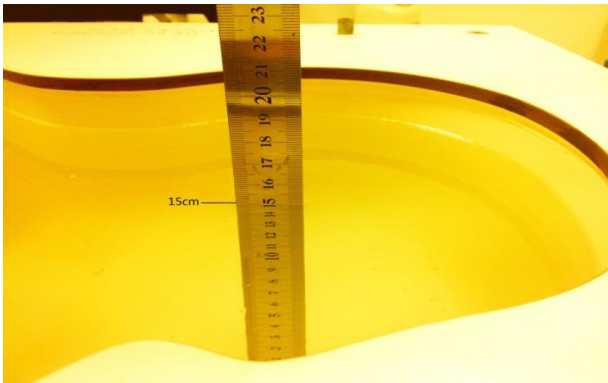
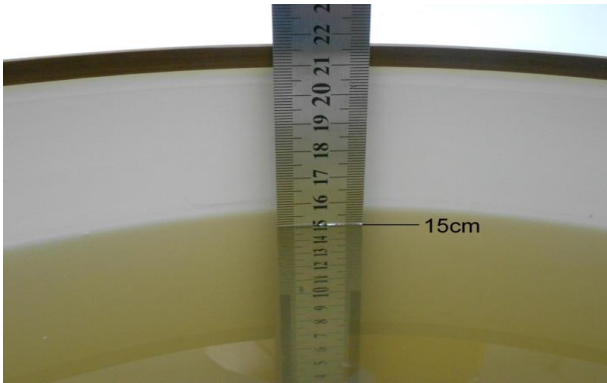
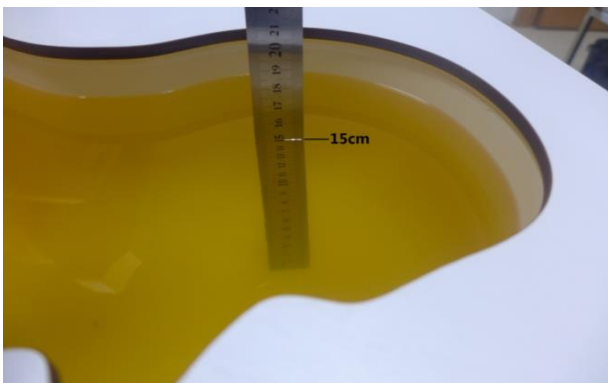
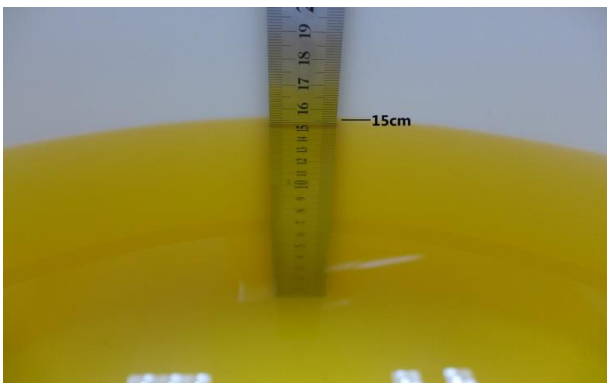
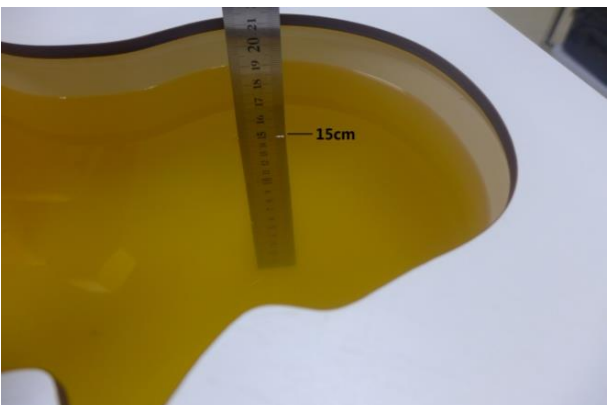
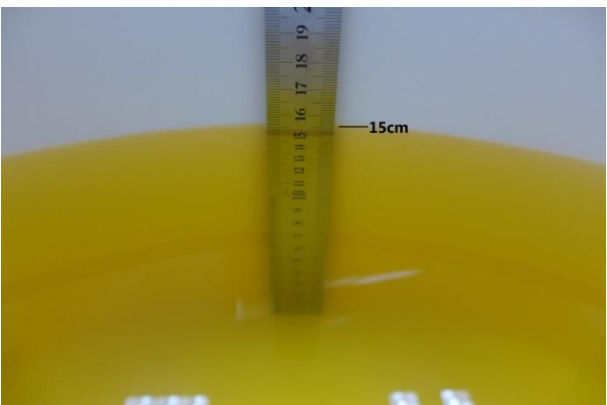
Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Body 1750
	
Photo 5: Tissue Simulant Liquid for Head 1900	Photo 6: Tissue Simulant Liquid for Body 1900
	

Photo 7: Tissue Simulant Liquid for Head 2450

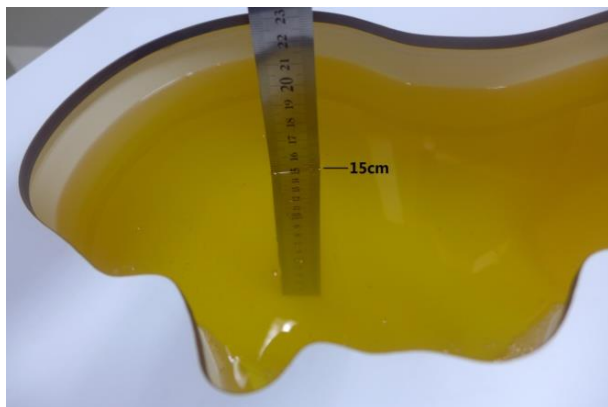


Photo 8: Tissue Simulant Liquid for Body 2450

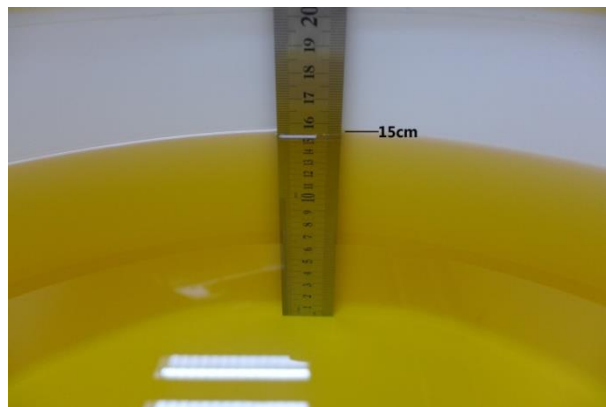


Photo 9: Tissue Simulant Liquid for Head 2600

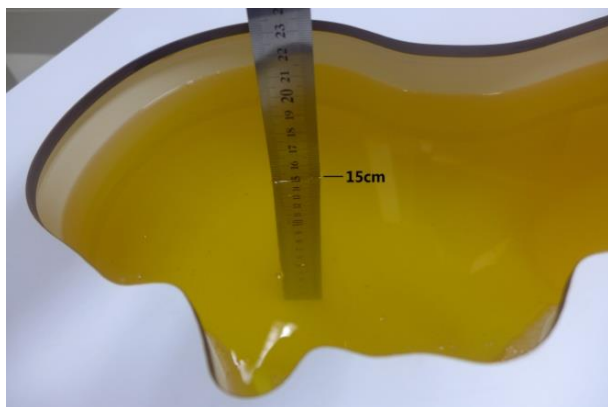


Photo 10: Tissue Simulant Liquid for Body 2600

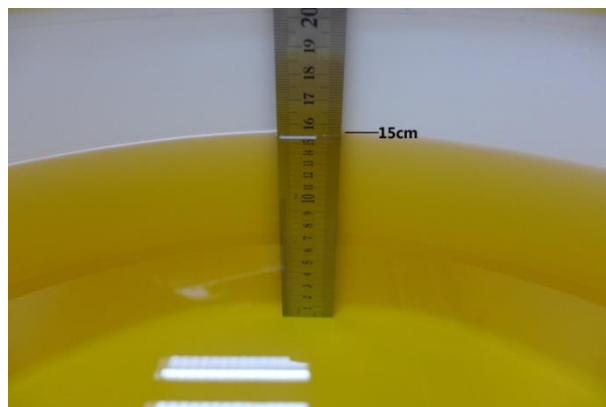


Photo 11: Tissue Simulant Liquid for Head 5G

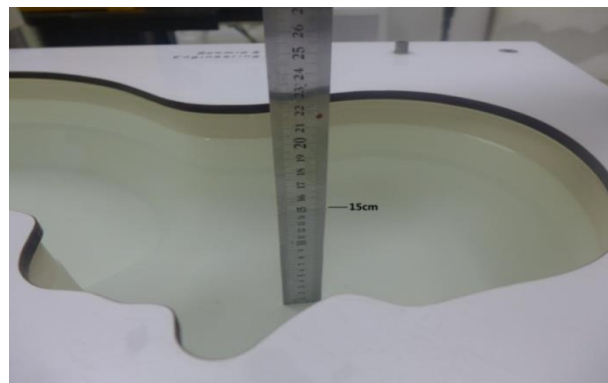
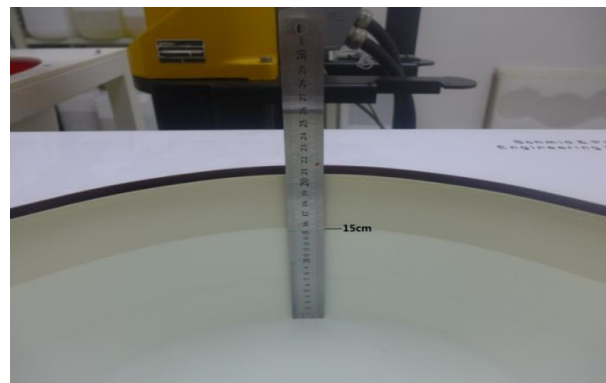


Photo 12: Tissue Simulant Liquid for Body 5G



3. Photographs of EUT test position

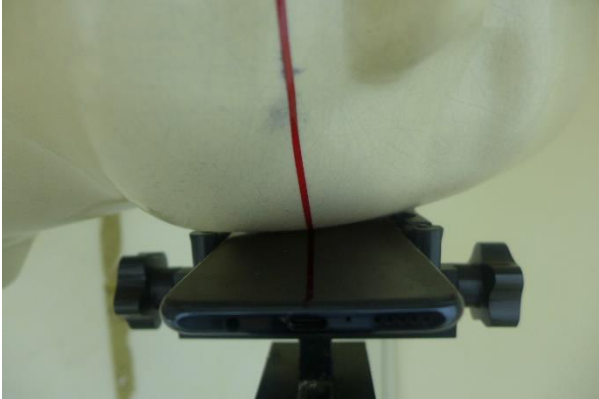
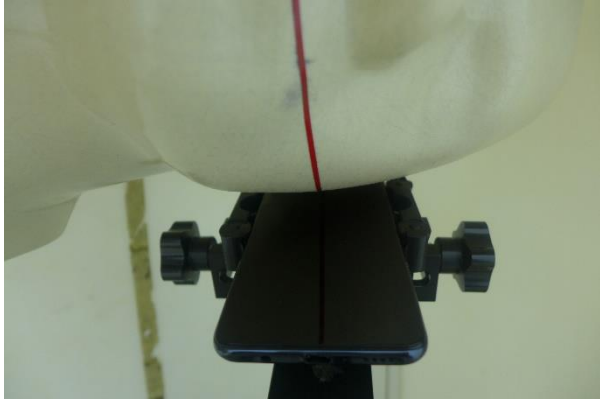
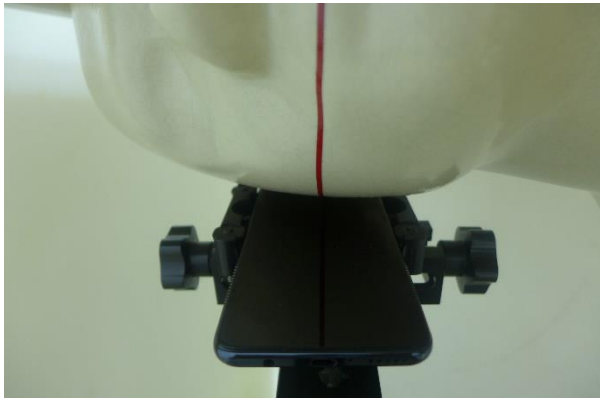
Photo 13: Left touch cheek	Photo 14: Left tilted 15 degree
	
Photo 15: Right touch cheek	Photo 16: Right tilted 15 degree
	
Photo 17: Front side 15mm	Photo 18: Back side 15mm
	

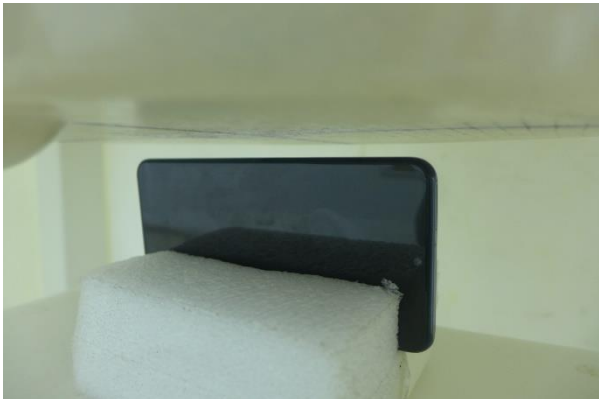
Photo 19: Front side 10mm	Photo 20: Back side 10mm
	
Photo 21: Left side 10mm	Photo 22: Right side 10mm
	
Photo 23: Top side 10mm	Photo 24: Bottom side 10mm
	

Photo 25: Front side 0mm	Photo 26: Back side 0mm
	
Photo 27: Right side 0mm	Photo 28: Top side 0mm
	

4. EUT Constructional Details

Photo 29: Front View	Photo 30: Back View
	
Photo 31: Accessory	NA
	NA